

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072921\
 Data File : PD064541.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jul 2021 08:19
 Operator : AR\AJ
 Sample : M3082-11
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0009

Manual Integrations
 APPROVED

mohammad
 7/30/2021 4:50:27 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 09:14:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 28 07:07:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	5.406	4.619	17996073	170.3E6	15.086	18.641
27)	SA Decachlor...	11.306	10.364	29663898	129.2E6	22.534m	21.720
Target Compounds							
3)	MA gamma-BHC...	6.394	5.735	1227852	48348154	0.783	4.240 #
5)	MB Aldrin	7.422	6.471	1714867	45072245	1.089m	4.285 #
13)	MA Dieldrin	8.549	7.740	1607231	37023194	1.078	4.610m#
15)	B Endosulfa...	9.040	8.341	3197185	25137377	2.462	4.355 #
16)	A 4,4'-DDD	8.950	8.175	15203920	38538641	12.386	6.691m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072921\
Data File : PD064541.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jul 2021 08:19
Operator : AR\AJ
Sample : M3082-11
Misc :
ALS Vial : 61 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 09:14:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 28 07:07:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

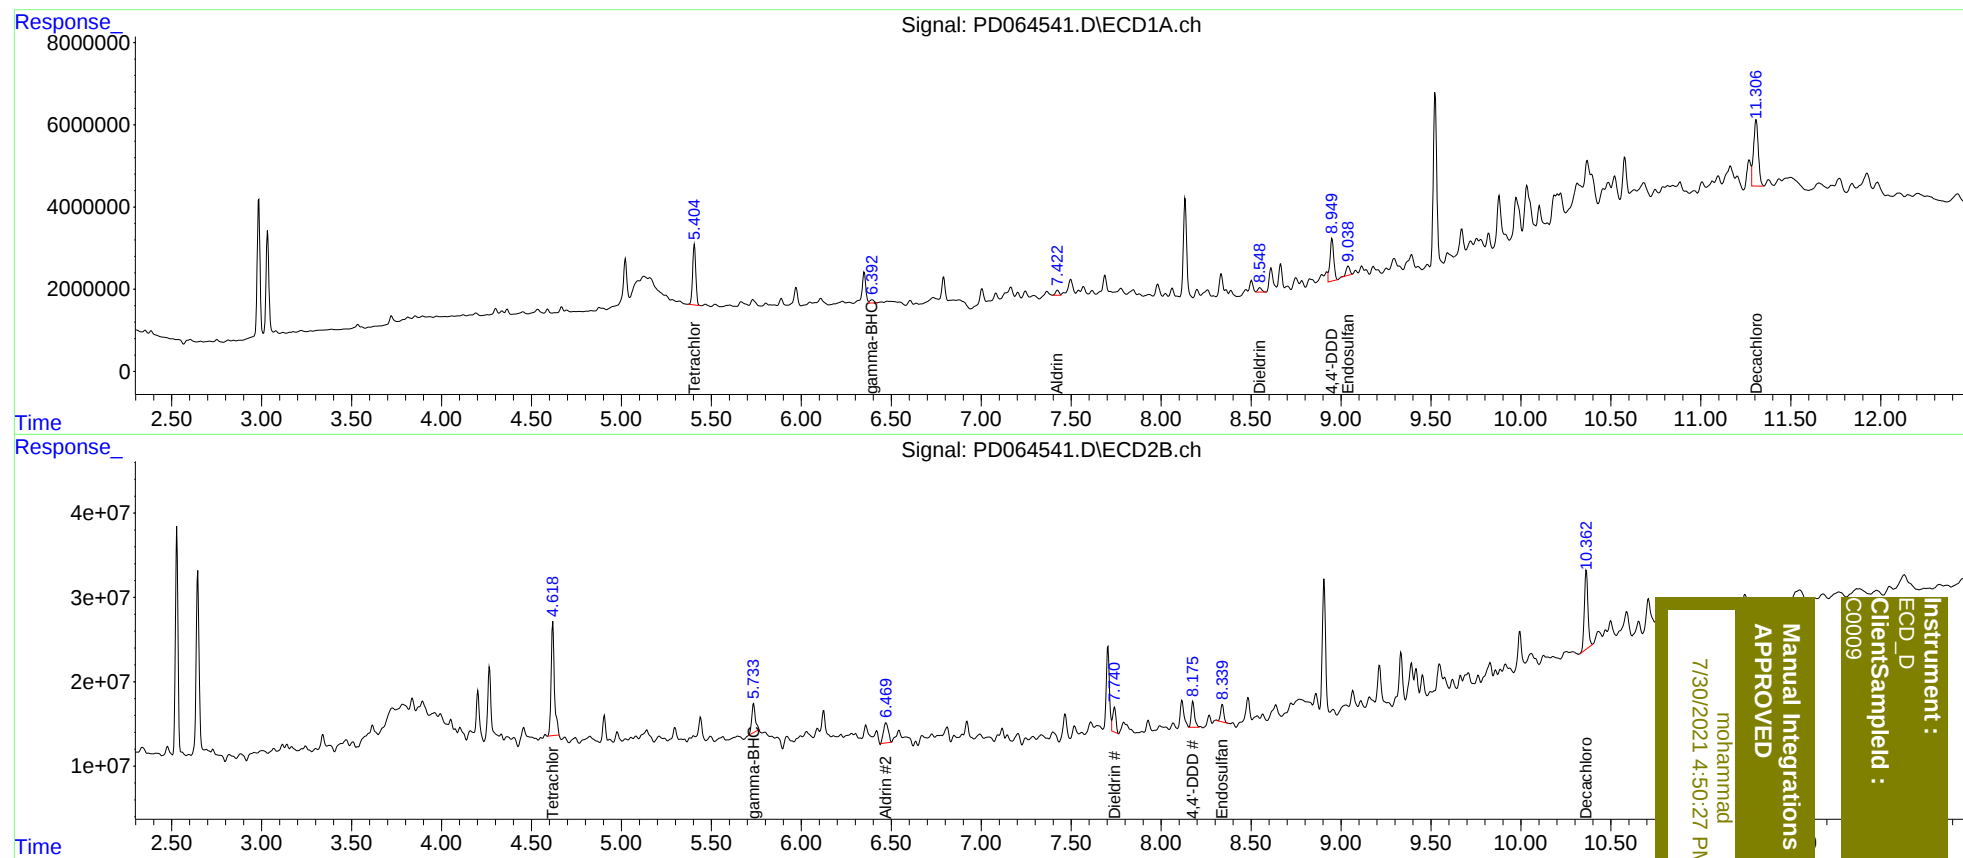

Instrument :
ECD_D
Client Sampled :
C0009

Manual Integrations
APPROVED
mohammad
7/30/2021 4:50:27 PM