

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072921\
 Data File : PD064525.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jul 2021 01:35
 Operator : AR\AJ
 Sample : M3082-06MS
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0005MS

Manual Integrations
 APPROVED

mohammad
 7/30/2021 4:49:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 06:57:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 28 07:07:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	5.406	4.619	18147206	150.7E6	15.213	16.496
27)	SA Decachlor...	11.314	10.361	77624570	214.6E6	58.968m	36.086 #
Target Compounds							
2)	A alpha-BHC	5.988	5.322	95162651	683.4E6	58.415	55.445
3)	MA gamma-BHC...	6.385	5.740	83829601	606.5E6	53.450	53.189m
4)	MA Heptachlor	7.035	6.151	76395198	536.6E6	45.457	47.331
5)	MB Aldrin	7.405	6.475	75355252	498.7E6	47.840	47.406
6)	B beta-BHC	6.644	6.117	33746148	225.7E6	43.255	37.205
7)	B delta-BHC	6.909	6.379	79173264	537.9E6	45.498	49.517
8)	B Heptachlo...	7.875	7.046	71768755	518.2E6	41.803	55.983m#
9)	A Endosulfan I	8.279	7.450	53501451	336.1E6	37.953	43.711m
10)	B trans-Chl...	8.143	7.323	111.7E6	514.0E6	69.677	56.667m
11)	B cis-Chlor...	8.227	7.394	63815013	416.4E6	40.957	46.814
12)	B 4,4'-DDE	8.421	7.606	122.8E6	624.9E6	85.233	82.824
13)	MA Dieldrin	8.571	7.735	155.2E6	573.8E6	104.049	71.438m#
14)	MA Endrin	8.809	8.026	120.7E6	512.0E6	94.288	89.130
15)	B Endosulfa...	9.043	8.335	126.1E6	449.9E6	97.096m	77.936
16)	A 4,4'-DDD	8.961	8.188	238.1E6	430.0E6	193.968m	74.659 #
17)	MA 4,4'-DDT	9.278	8.444	112.3E6	887.2E6	86.038m	161.174m#
18)	B Endrin al...	9.180	8.521	98407260	347.4E6	86.862	70.399m
19)	B Endosulfa...	9.418	8.753	113.1E6	586.0E6	82.072	108.712 #
20)	A Methoxychlor	9.770	9.040	300.4E6	770.9E6	419.859m	301.058m#
21)	B Endrin ke...	9.915	9.271	129.8E6	298.8E6	85.768	49.815 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072921\
Data File : PD064525.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jul 2021 01:35
Operator : AR\AJ
Sample : M3082-06MS
Misc :
ALS Vial : 45 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 06:57:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 28 07:07:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

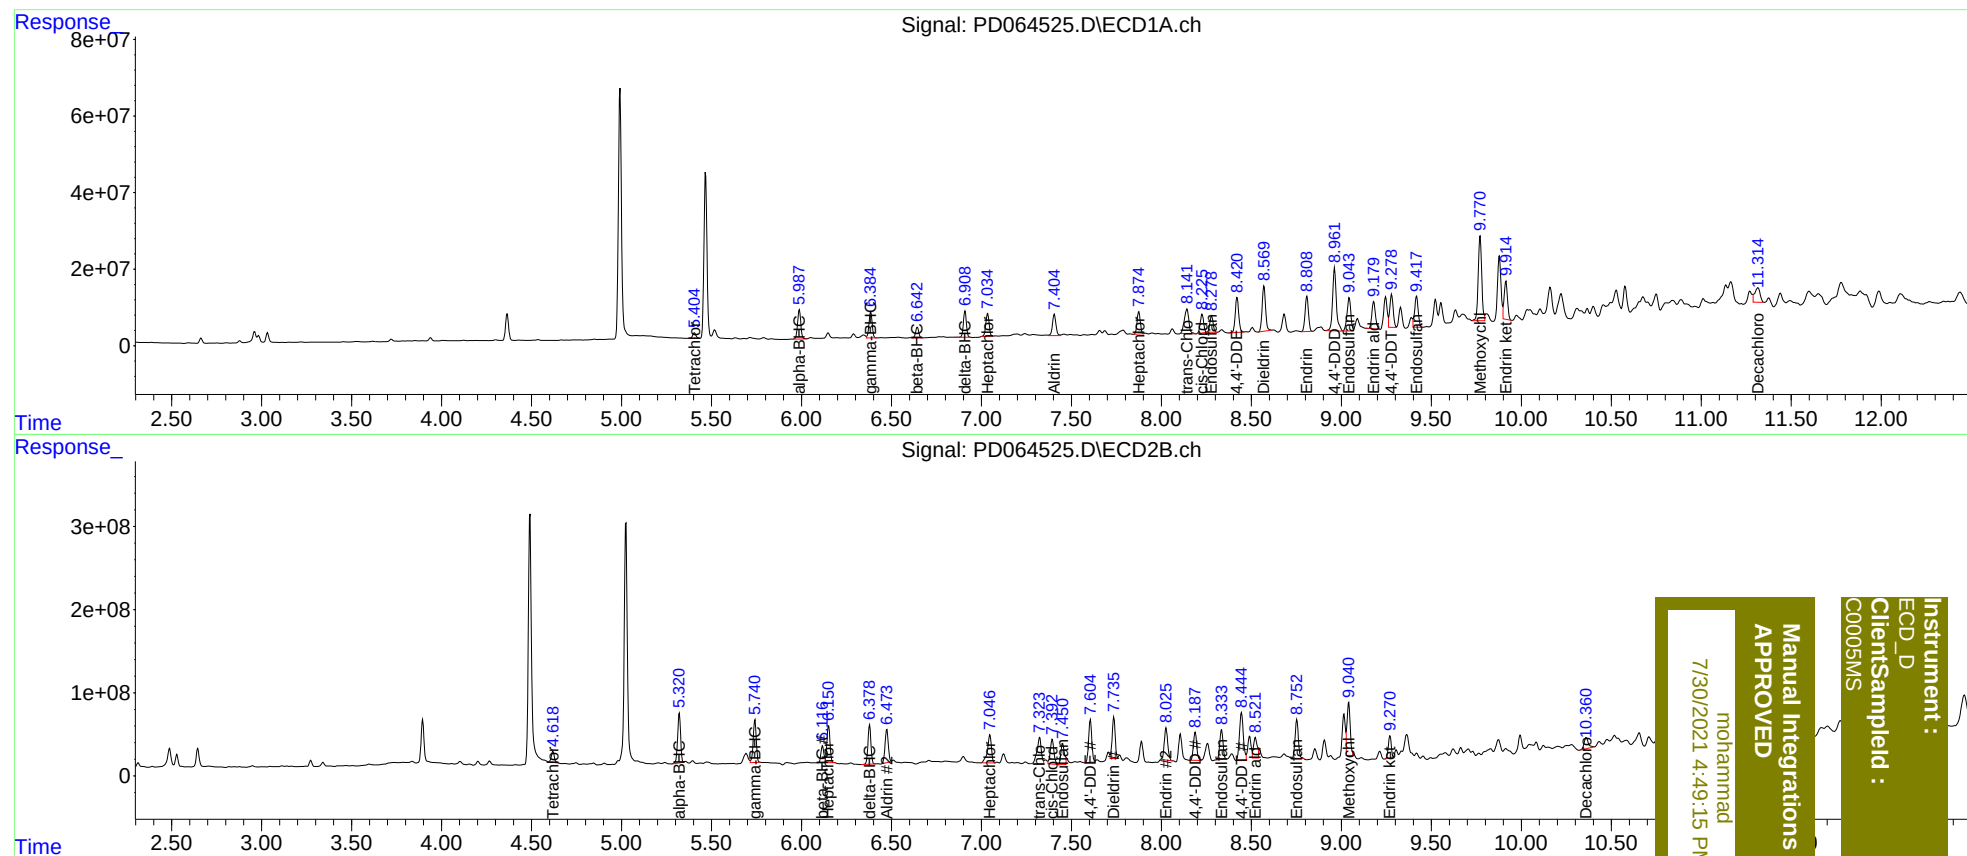

Manual Integrations
APPROVED

mohammad
7/30/2021 4:49:15 PM

Instrument :
ECD_D
Client Sampled :
C0005MS