

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072921\
 Data File : PD064526.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jul 2021 02:07
 Operator : AR\AJ
 Sample : M3082-07MSD
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0005MSD

Manual Integrations
 APPROVED

mohammad
 7/30/2021 4:49:45 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 06:58:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 28 07:07:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	5.406	4.620	19638627	156.0E6	16.463	17.077
27)	SA Decachlor...	11.313	10.361	80137772	206.0E6	60.877m	34.634 #
Target Compounds							
2)	A alpha-BHC	5.989	5.322	98094265	693.5E6	60.214	56.268
3)	MA gamma-BHC...	6.385	5.741	85231928	604.5E6	54.345	53.012m
4)	MA Heptachlor	7.036	6.152	76226490	540.5E6	45.357	47.673
5)	MB Aldrin	7.404	6.474	71880662	554.2E6	45.634m	52.687m
6)	B beta-BHC	6.644	6.118	33813297	227.8E6	43.341	37.555
7)	B delta-BHC	6.910	6.379	81037258	544.6E6	46.569	50.132
8)	B Heptachlo...	7.875	7.047	73795205	482.3E6	42.983	52.104m
9)	A Endosulfan I	8.280	7.450	53322838	324.0E6	37.827	42.135m
10)	B trans-Chl...	8.142	7.323	113.9E6	516.5E6	71.049	56.941m
11)	B cis-Chlor...	8.227	7.394	63152499	415.9E6	40.532	46.750
12)	B 4,4'-DDE	8.422	7.606	127.3E6	606.1E6	88.300	80.330
13)	MA Dieldrin	8.571	7.735	161.0E6	612.2E6	107.945	76.224m#
14)	MA Endrin	8.809	8.027	122.6E6	501.9E6	95.762	87.375
15)	B Endosulfa...	9.043	8.335	126.9E6	447.2E6	97.749m	77.477
16)	A 4,4'-DDD	8.962	8.188	256.1E6	455.0E6	208.626m	79.004m#
17)	MA 4,4'-DDT	9.279	8.444	122.4E6	855.2E6	93.789m	155.364m#
18)	B Endrin al...	9.181	8.521	97393179	338.0E6	85.967	68.491m
19)	B Endosulfa...	9.419	8.753	109.5E6	591.0E6	79.484	109.641 #
20)	A Methoxychlor	9.771	9.040	302.2E6	801.2E6	422.395m	312.913m#
21)	B Endrin ke...	9.915	9.270	133.1E6	293.1E6	87.978	48.858 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072921\
Data File : PD064526.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jul 2021 02:07
Operator : AR\AJ
Sample : M3082-07MSD
Misc :
ALS Vial : 46 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 06:58:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 28 07:07:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

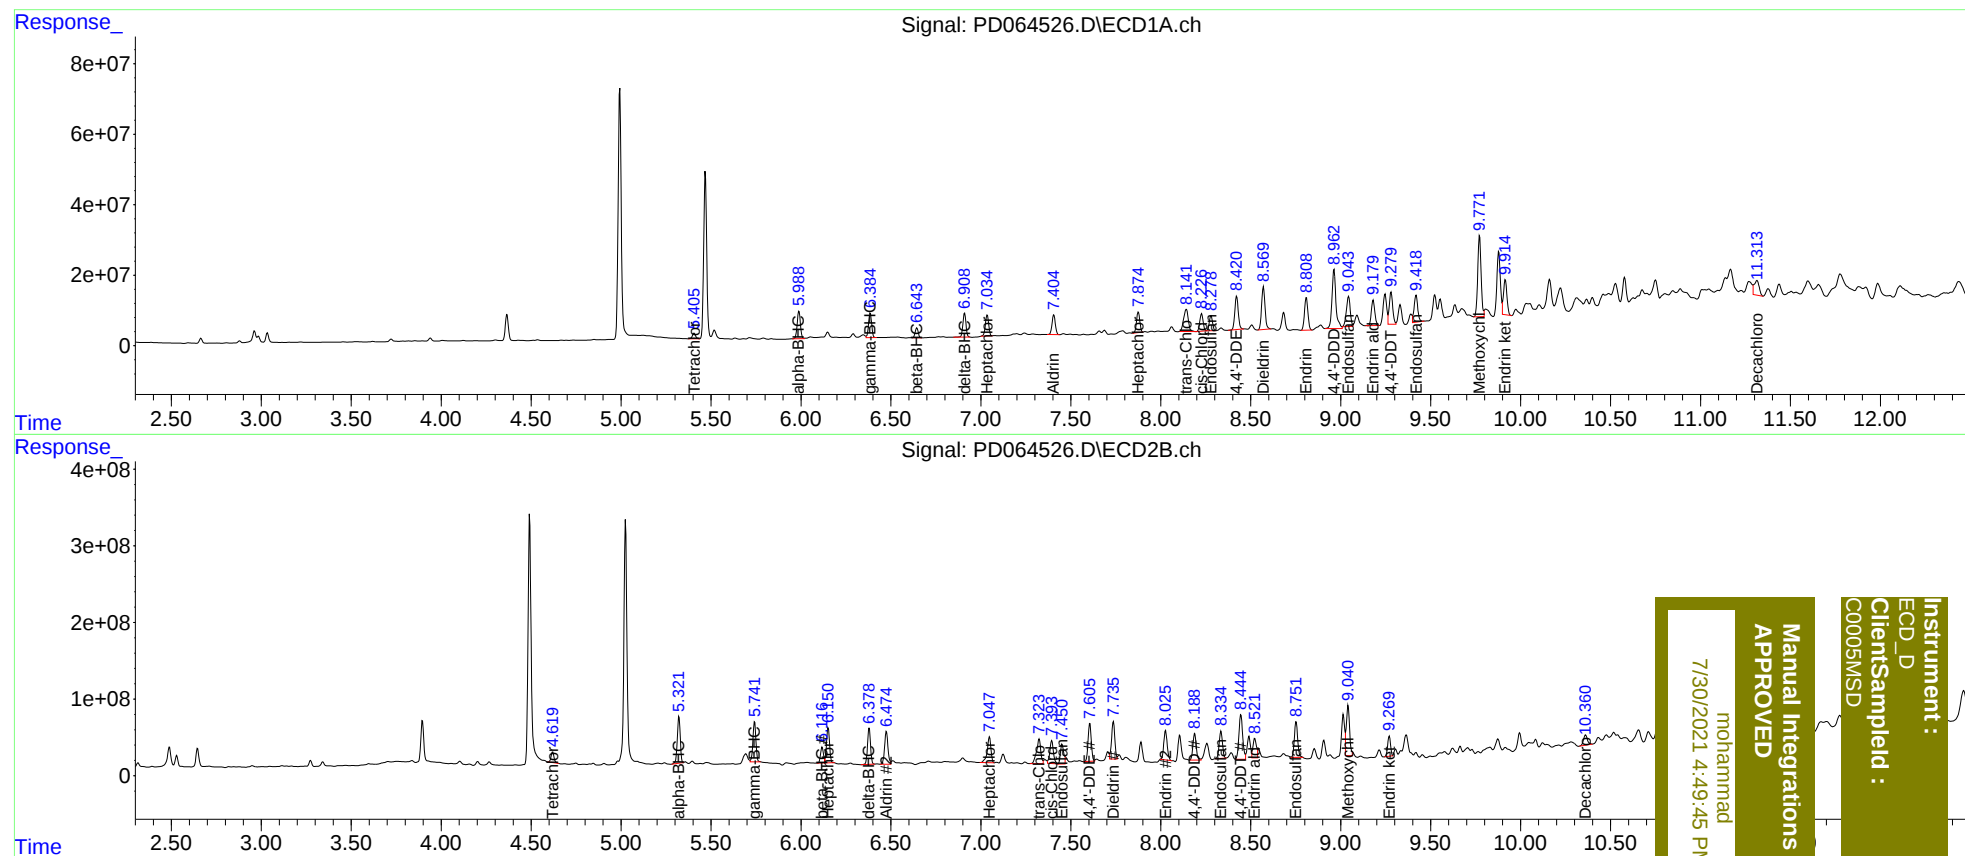

Manual Integrations
APPROVED

7/30/2021 4:49:45 PM
mohammad

Instrument :
ECD_D
Client Sample :
C0005MSD