

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072924\
 Data File : PD084127.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2024 13:33
 Operator : AR\AJ
 Sample : P3379-07
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 OU4-PCS-04-072324

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 02:41:05 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071524.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 16 04:22:06 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.561	2.770	19482308	117.0E6	19.054	20.357
28)	SA Decachlor...	9.117	7.896	37757077	117.3E6	16.539	18.266

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072924\
Data File : PD084127.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2024 13:33
Operator : AR\AJ
Sample : P3379-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
OU4-PCS-04-072324

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 02:41:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071524.M
Quant Title : GC Extractables
QLast Update : Tue Jul 16 04:22:06 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

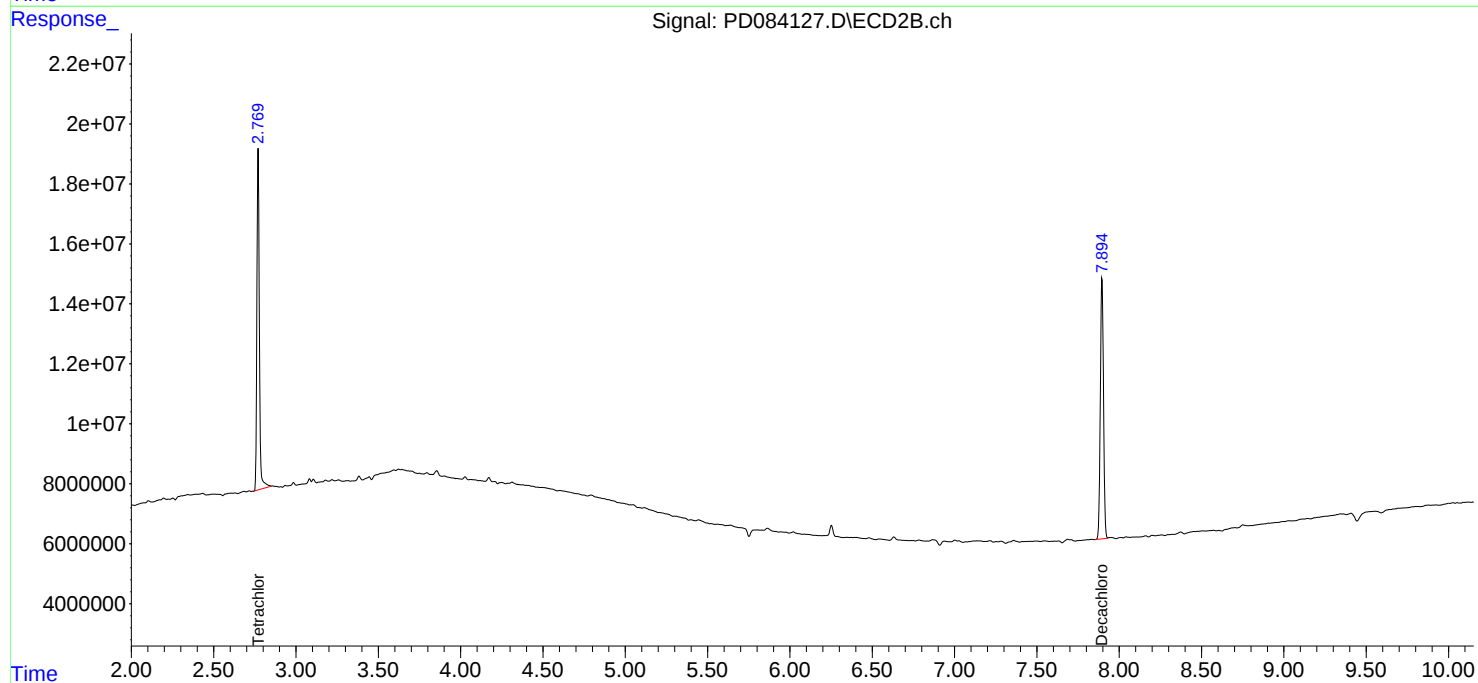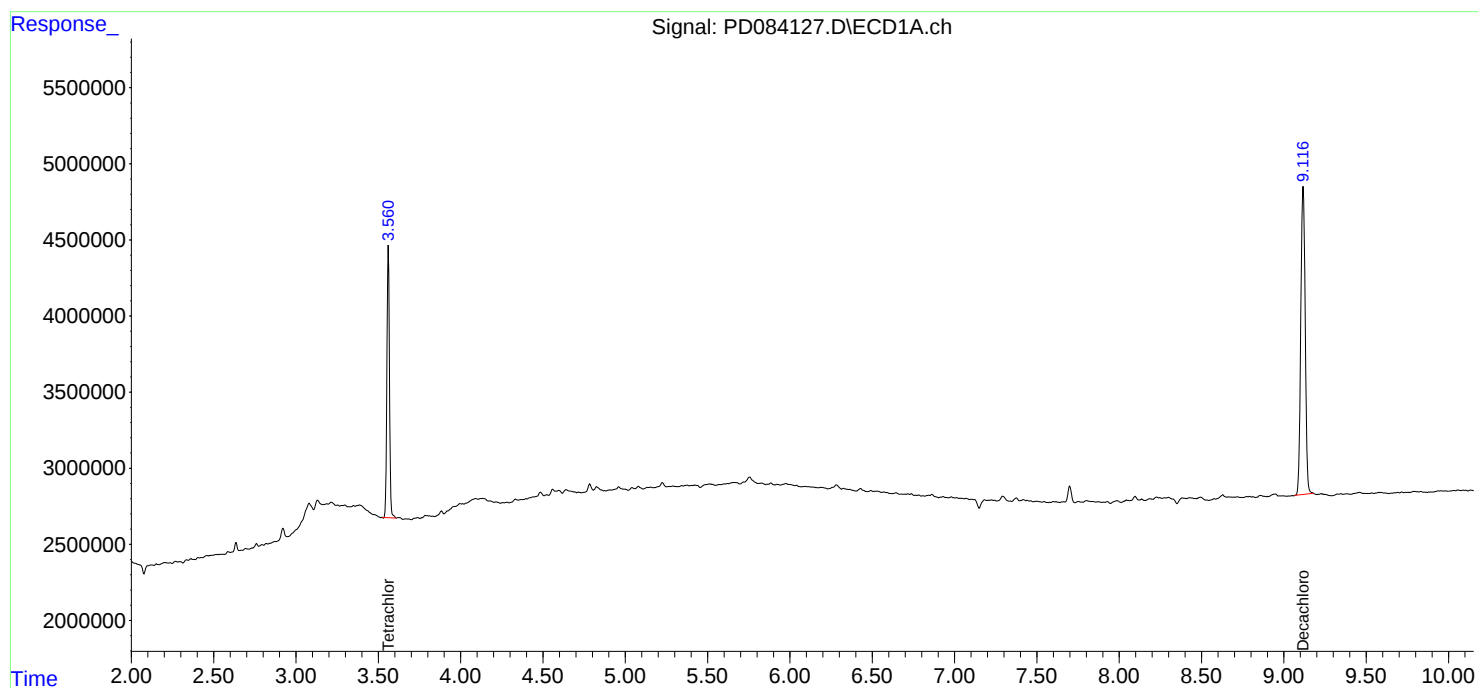


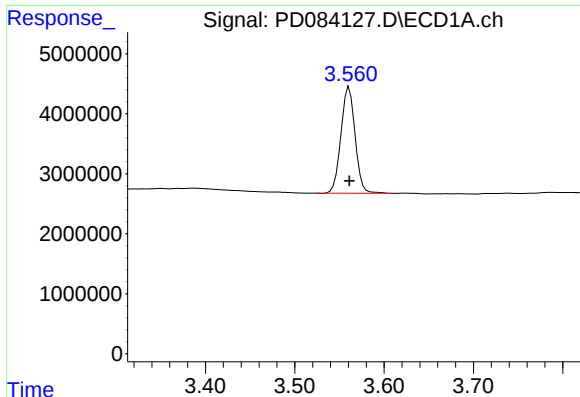

#1 Tetrachloro-m-xylene


R.T.: 3.561 min
Delta R.T.: 0.000 min
Response: 19482308
Conc: 19.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
OU4-PCS-04-072324

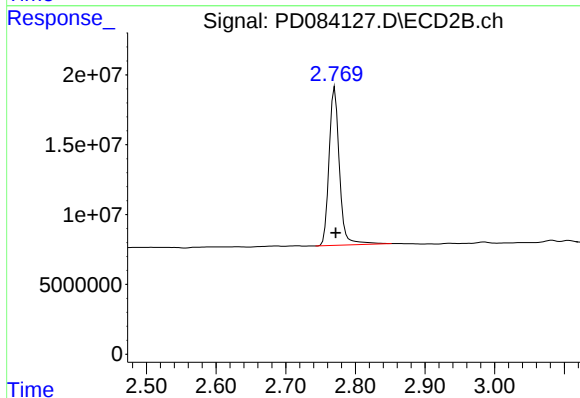


#1 Tetrachloro-m-xylene

R.T.: 2.770 min
Delta R.T.: -0.001 min
Response: 117043531
Conc: 20.36 ng/ml

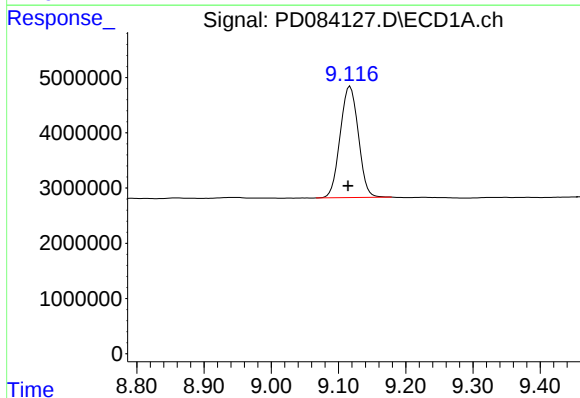

#28 Decachlorobiphenyl

R.T.: 9.117 min
Delta R.T.: 0.003 min
Response: 37757077
Conc: 16.54 ng/ml

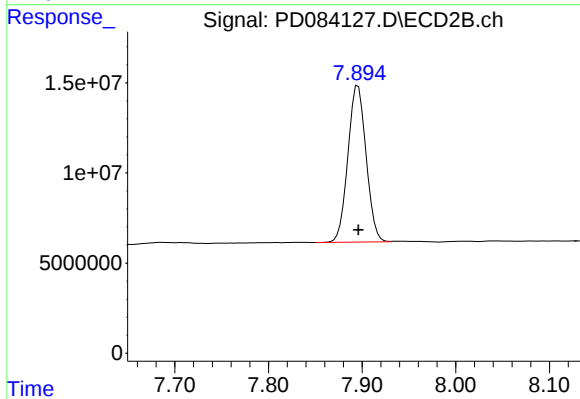

#28 Decachlorobiphenyl

R.T.: 7.896 min
Delta R.T.: 0.000 min
Response: 117303151
Conc: 18.27 ng/ml