

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072924\
 Data File : PD084133.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2024 15:36
 Operator : AR\AJ
 Sample : P3379-17
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 OU4-VSL-04-072324

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/30/2024
 Supervised By :Ankita Jodhani 07/30/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 02:42:39 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071524.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 16 04:22:06 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.568	2.770	15057200	91189918	14.726m	15.860
28) SA Decachlor...	9.128	7.898	30621774	95337622	13.414	14.845

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072924\
Data File : PD084133.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2024 15:36
Operator : AR\AJ
Sample : P3379-17
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
OU4-VSL-04-072324


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/30/2024
Supervised By : Ankita Jodhani 07/30/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 02:42:39 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071524.M
Quant Title : GC Extractables
QLast Update : Tue Jul 16 04:22:06 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

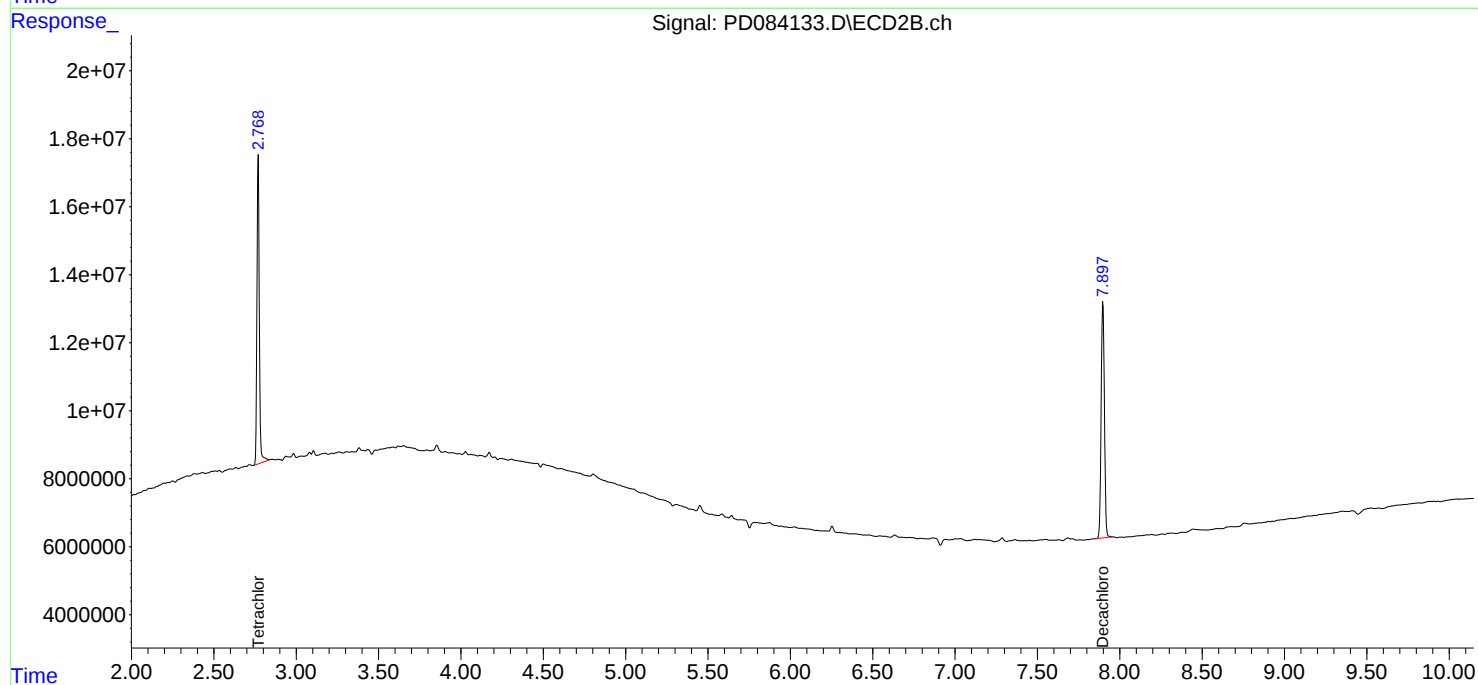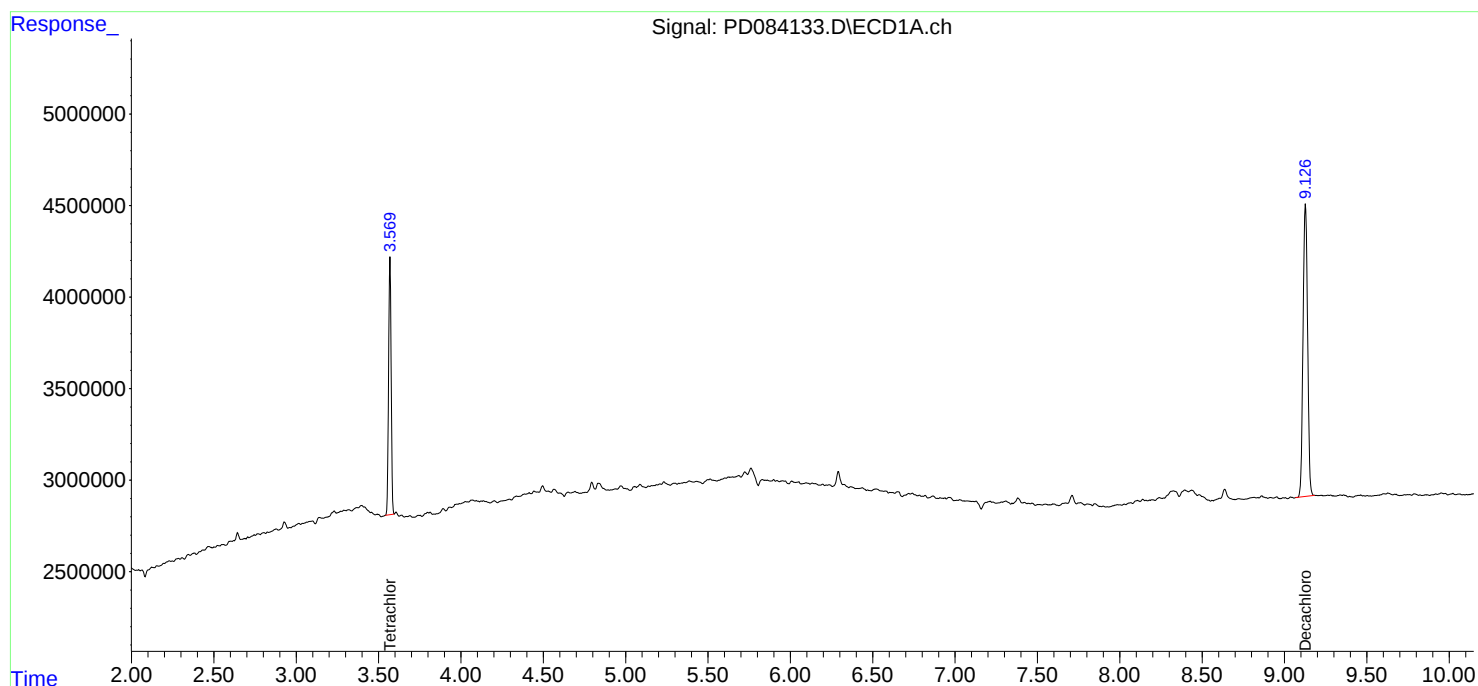

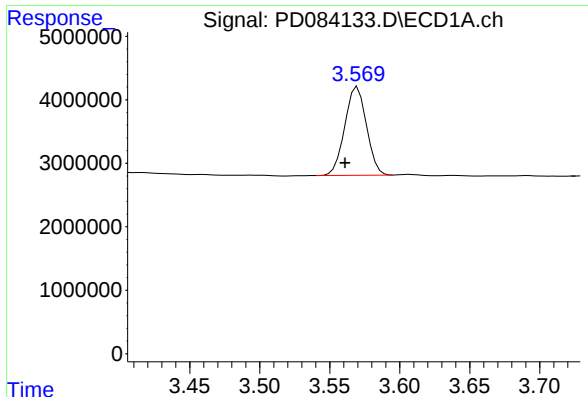

#1 Tetrachloro-m-xylene

R.T.: 3.568 min
Delta R.T.: 0.007 min
Response: 15057200
Conc: 14.73 ng/ml

Instrument :

ECD_D


ClientSampleId :

OU4-VSL-04-072324

Manual Integrations


APPROVED

Reviewed By :Abdul Mirza 07/30/2024
Supervised By :Ankita Jodhani 07/30/2024

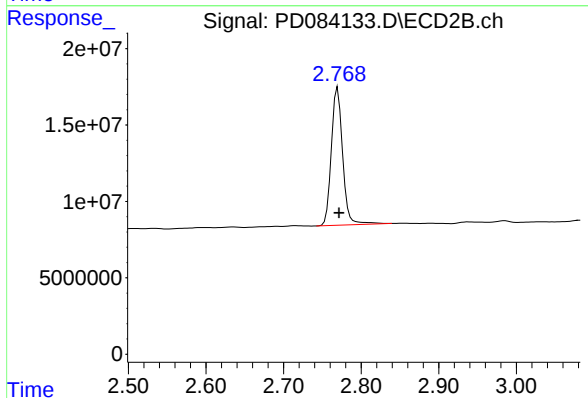


#1 Tetrachloro-m-xylene

R.T.: 2.770 min
Delta R.T.: -0.002 min
Response: 91189918
Conc: 15.86 ng/ml

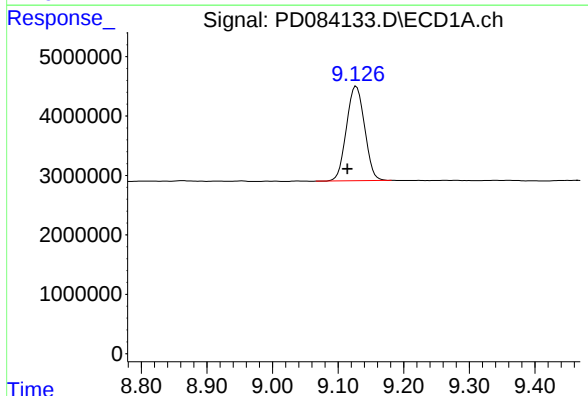

#28 Decachlorobiphenyl

R.T.: 9.128 min
Delta R.T.: 0.013 min
Response: 30621774
Conc: 13.41 ng/ml

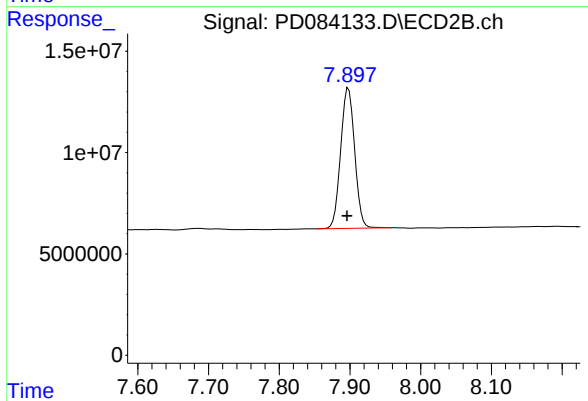

#28 Decachlorobiphenyl

R.T.: 7.898 min
Delta R.T.: 0.002 min
Response: 95337622
Conc: 14.85 ng/ml