

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073019\
 Data File : PD054106.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Jul 2019 8:49
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 02:32:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071819CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 07:29:30 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

8) B	Heptachlo...	5.028f	0.000	1572453	0	1.935	N.D.	#
9) A	Endosulfan I	5.282f	0.000	1576002	0	2.021	N.D.	#
11) B	cis-Chlor...	5.282	0.000	1576002	0	1.887	N.D.	#


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073019\
Data File : PD054106.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Jul 2019 8:49
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 02:32:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071819CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 07:29:30 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

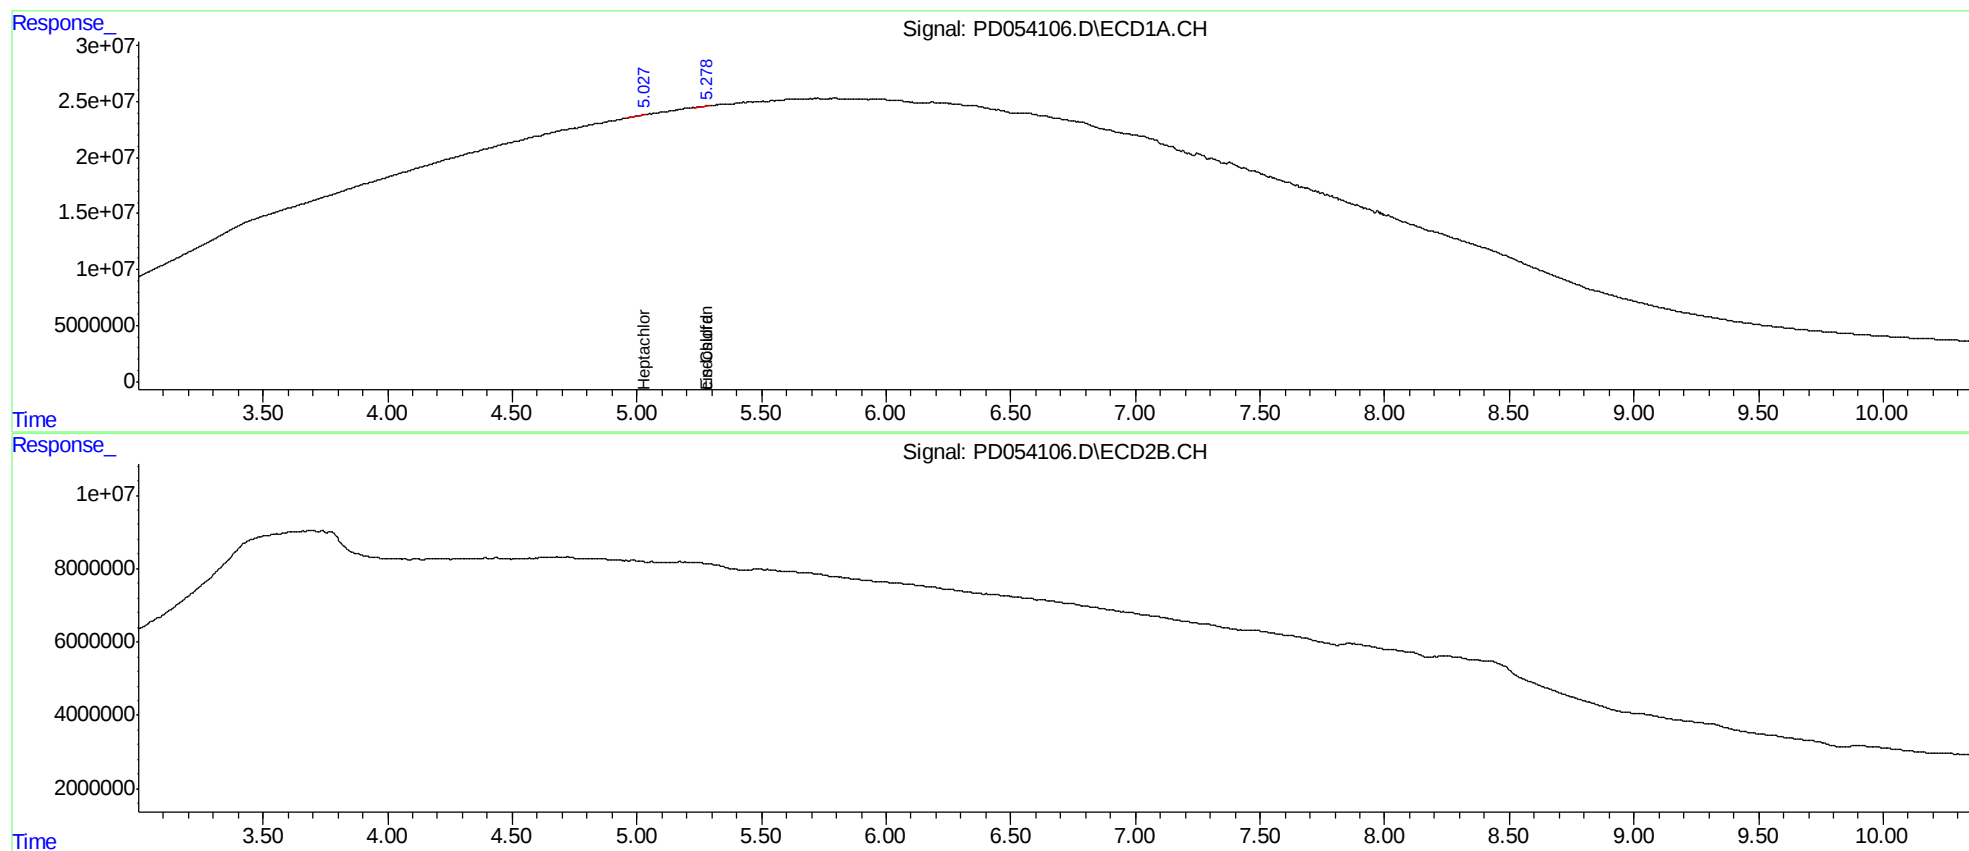


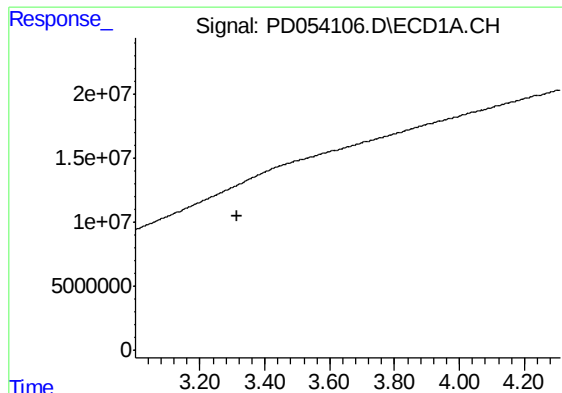

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.313 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

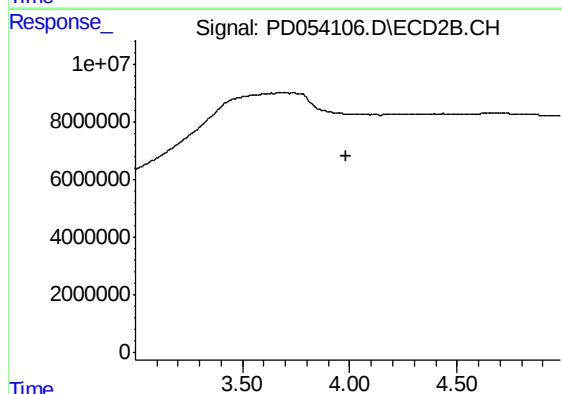


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.983 min
Response: 0
Conc: N.D.

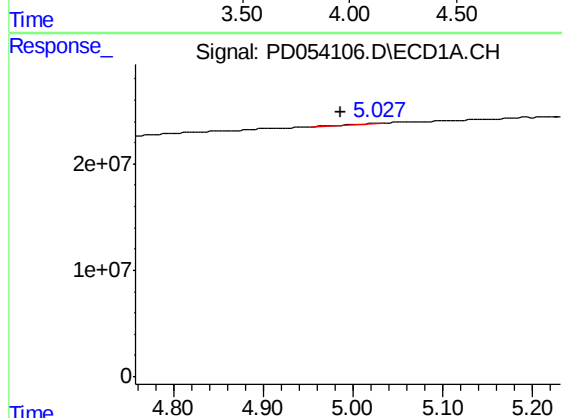


#8 Heptachlor epoxide

R.T.: 5.028 min
Delta R.T.: 0.042 min
Response: 1572453
Conc: 1.94 ng/ml

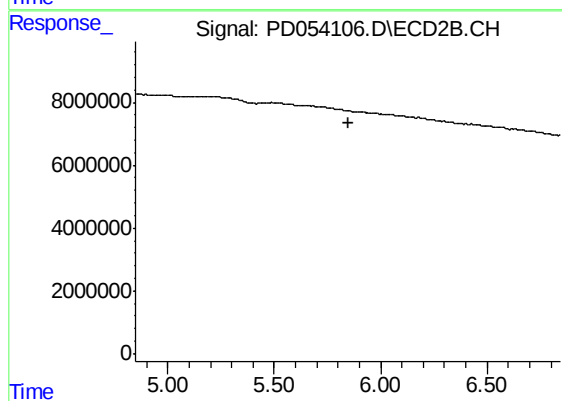

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.848 min
Response: 0
Conc: N.D.

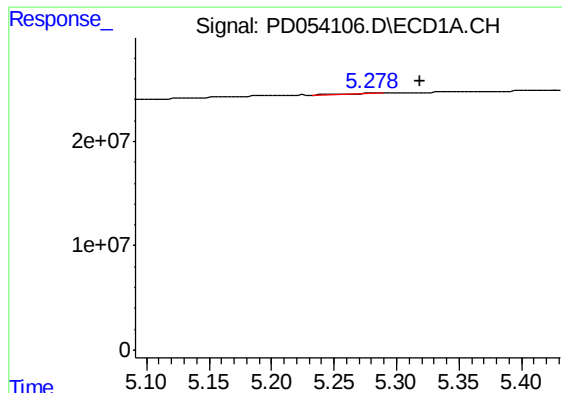

#9 Endosulfan I


R.T.: 5.282 min
Delta R.T.: -0.037 min
Response: 1576002
Conc: 2.02 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

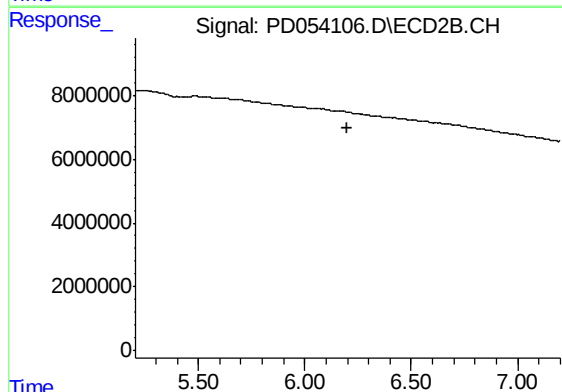


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.203 min
Response: 0
Conc: N.D.

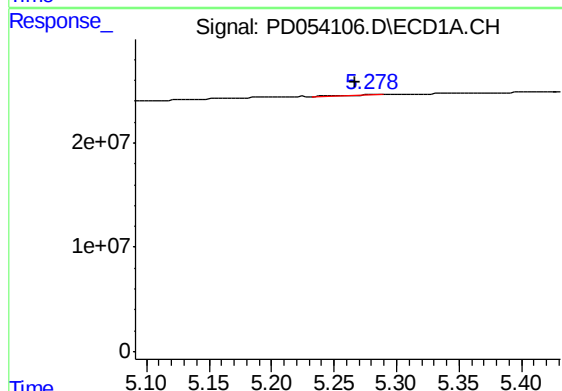


#11 cis-Chlordane

R.T.: 5.282 min
Delta R.T.: 0.014 min
Response: 1576002
Conc: 1.89 ng/ml

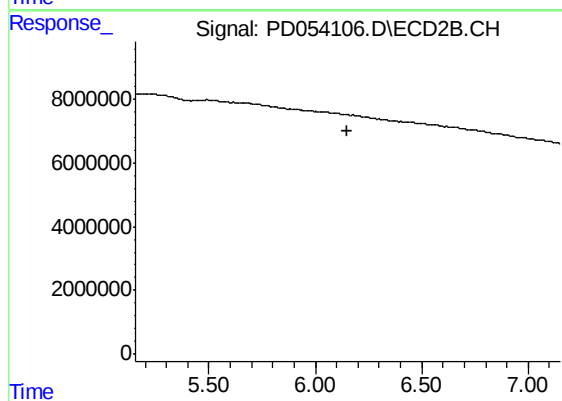

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.153 min
Response: 0
Conc: N.D.

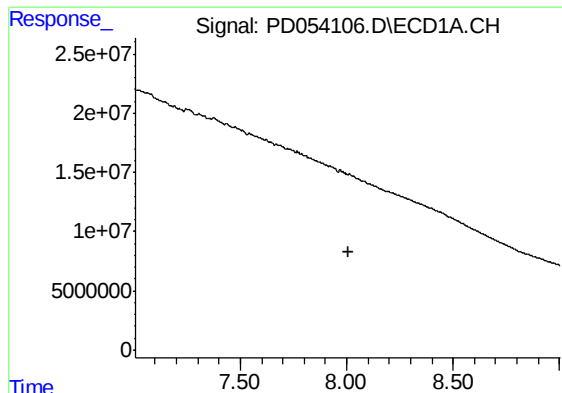

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.008 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

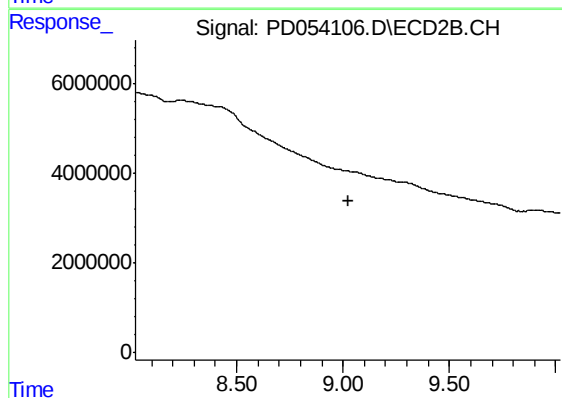

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.024 min
Response: 0
Conc: N.D.