

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073019\
 Data File : PD054141.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Jul 2019 17:45
 Operator : SM\AJ
 Sample : K3935-09
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BEP27

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 02:39:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071819CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 07:29:30 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.312	3.983	6436613	9407226	10.464	10.265
27) SA Decachlor...	8.007	9.024	9663917	13428293	13.801	14.303
Target Compounds						
6) B beta-BHC	4.229f	0.000	2915201	0	7.365	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073019\
Data File : PD054141.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Jul 2019 17:45
Operator : SM\AJ
Sample : K3935-09
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :
BEP27

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 02:39:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071819CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 07:29:30 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

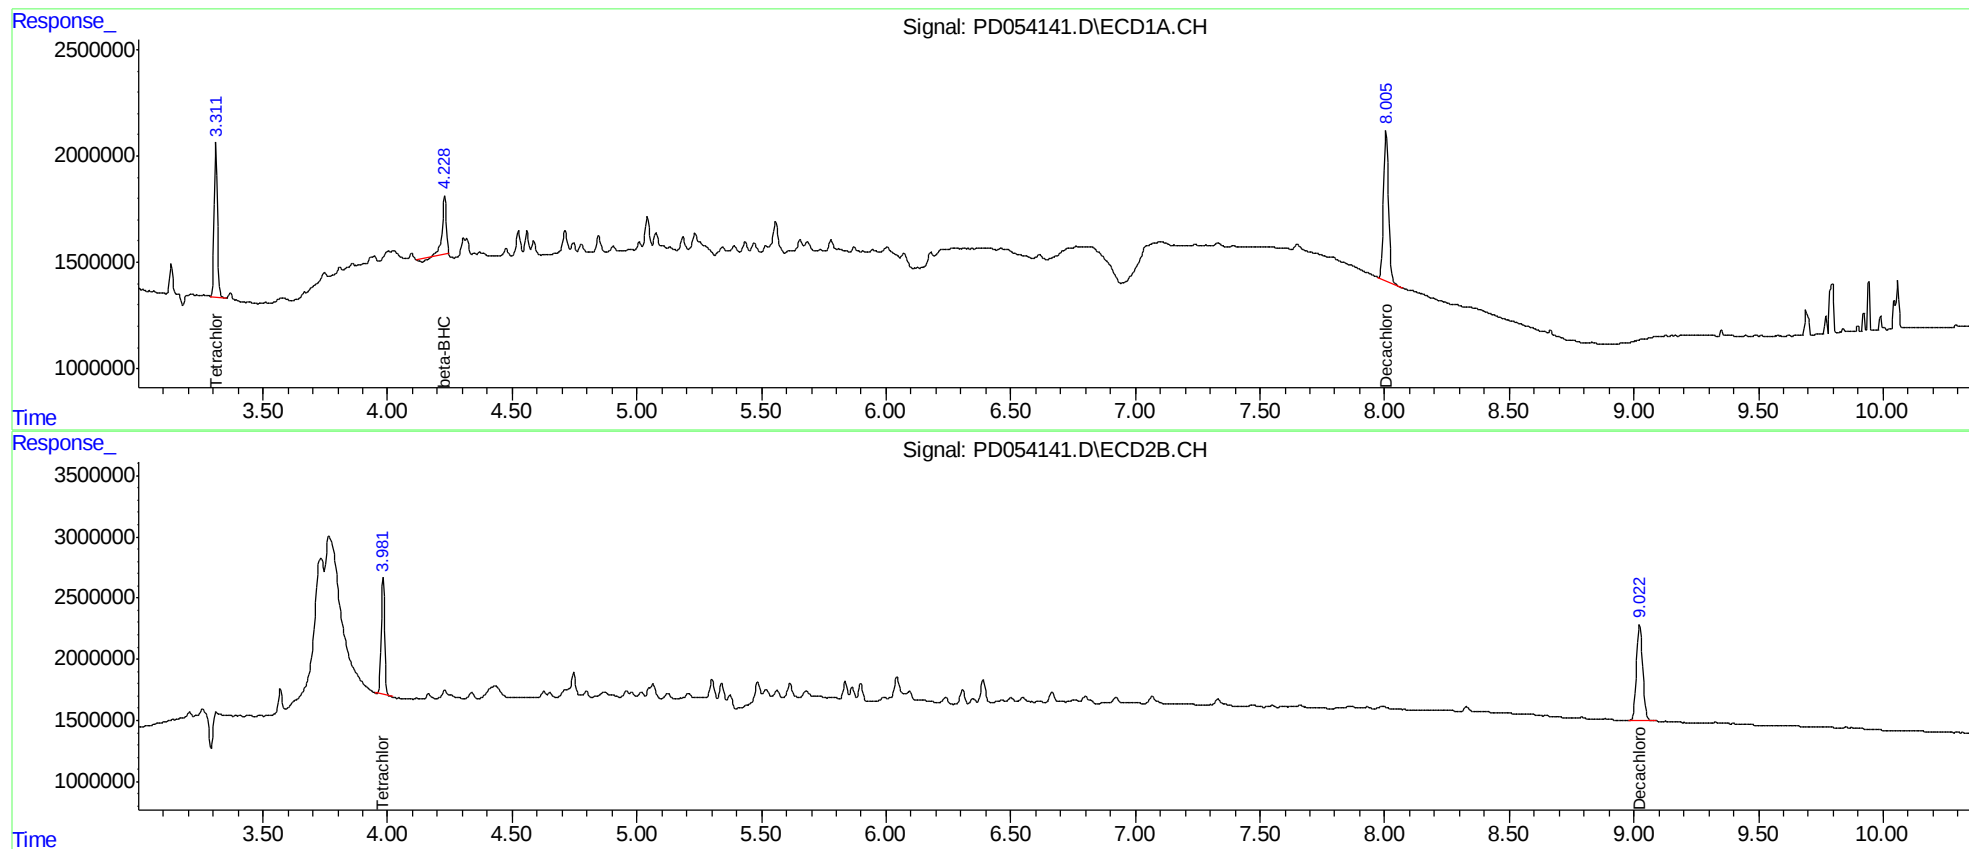


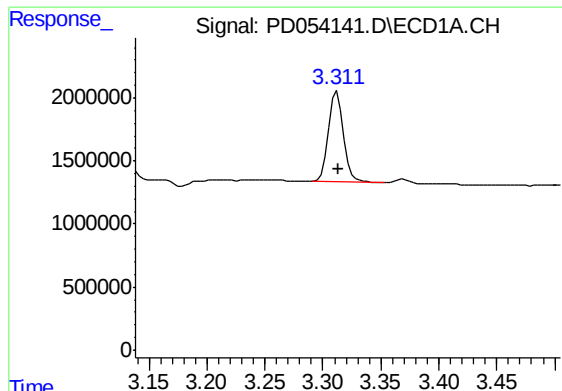

#1 Tetrachloro-m-xylene


R.T.: 3.312 min
Delta R.T.: 0.000 min
Response: 6436613
Conc: 10.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
BEP27

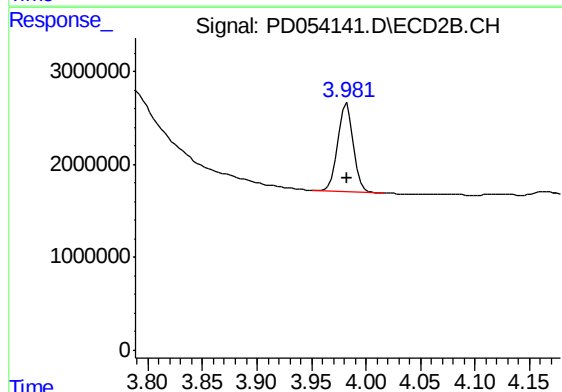


#1 Tetrachloro-m-xylene

R.T.: 3.983 min
Delta R.T.: 0.000 min
Response: 9407226
Conc: 10.27 ng/ml

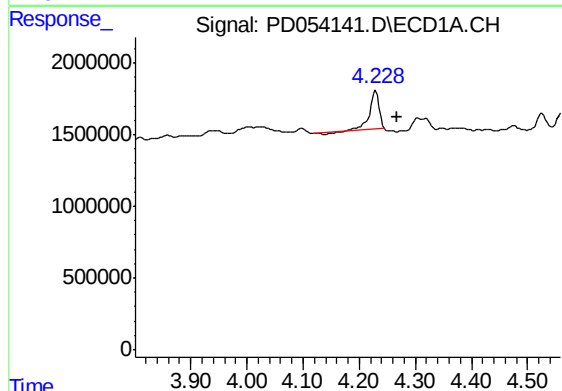


#6 beta-BHC

R.T.: 4.229 min
Delta R.T.: -0.038 min
Response: 2915201
Conc: 7.37 ng/ml

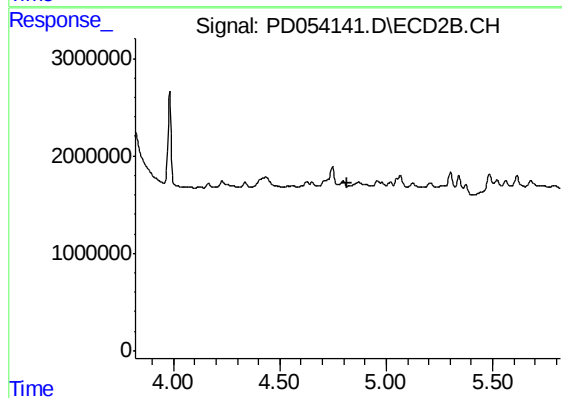

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.819 min
Response: 0
Conc: N.D.

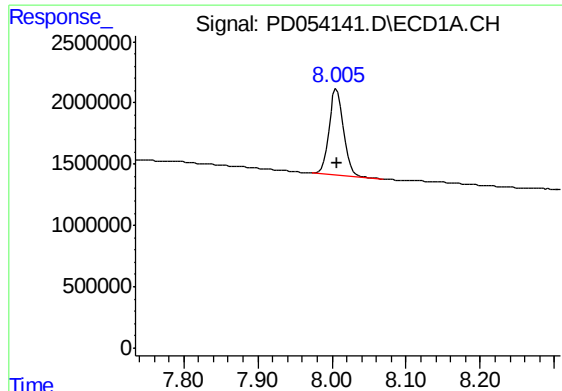

#27 Decachlorobiphenyl

R.T.: 8.007 min
Delta R.T.: -0.001 min
Response: 9663917
Conc: 13.80 ng/ml

Instrument :
ECD_D
ClientSampleId :
BEP27

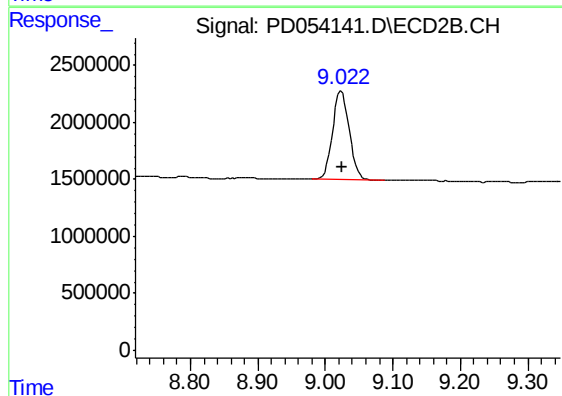

#27 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: 0.000 min
Response: 13428293
Conc: 14.30 ng/ml