

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073019\
 Data File : PD054142.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Jul 2019 17:58
 Operator : SM\AJ
 Sample : K3935-10
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BEP28

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 02:39:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071819CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 07:29:30 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.312	3.982	7412234	10979206	12.050	11.980
27)	SA Decachlor...	8.006	9.024	11877483	16104607	16.962	17.154
Target Compounds							
6)	B beta-BHC	4.230f	0.000	4250409	0	10.739	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073019\
Data File : PD054142.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Jul 2019 17:58
Operator : SM\AJ
Sample : K3935-10
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
BEP28

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 02:39:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071819CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 07:29:30 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

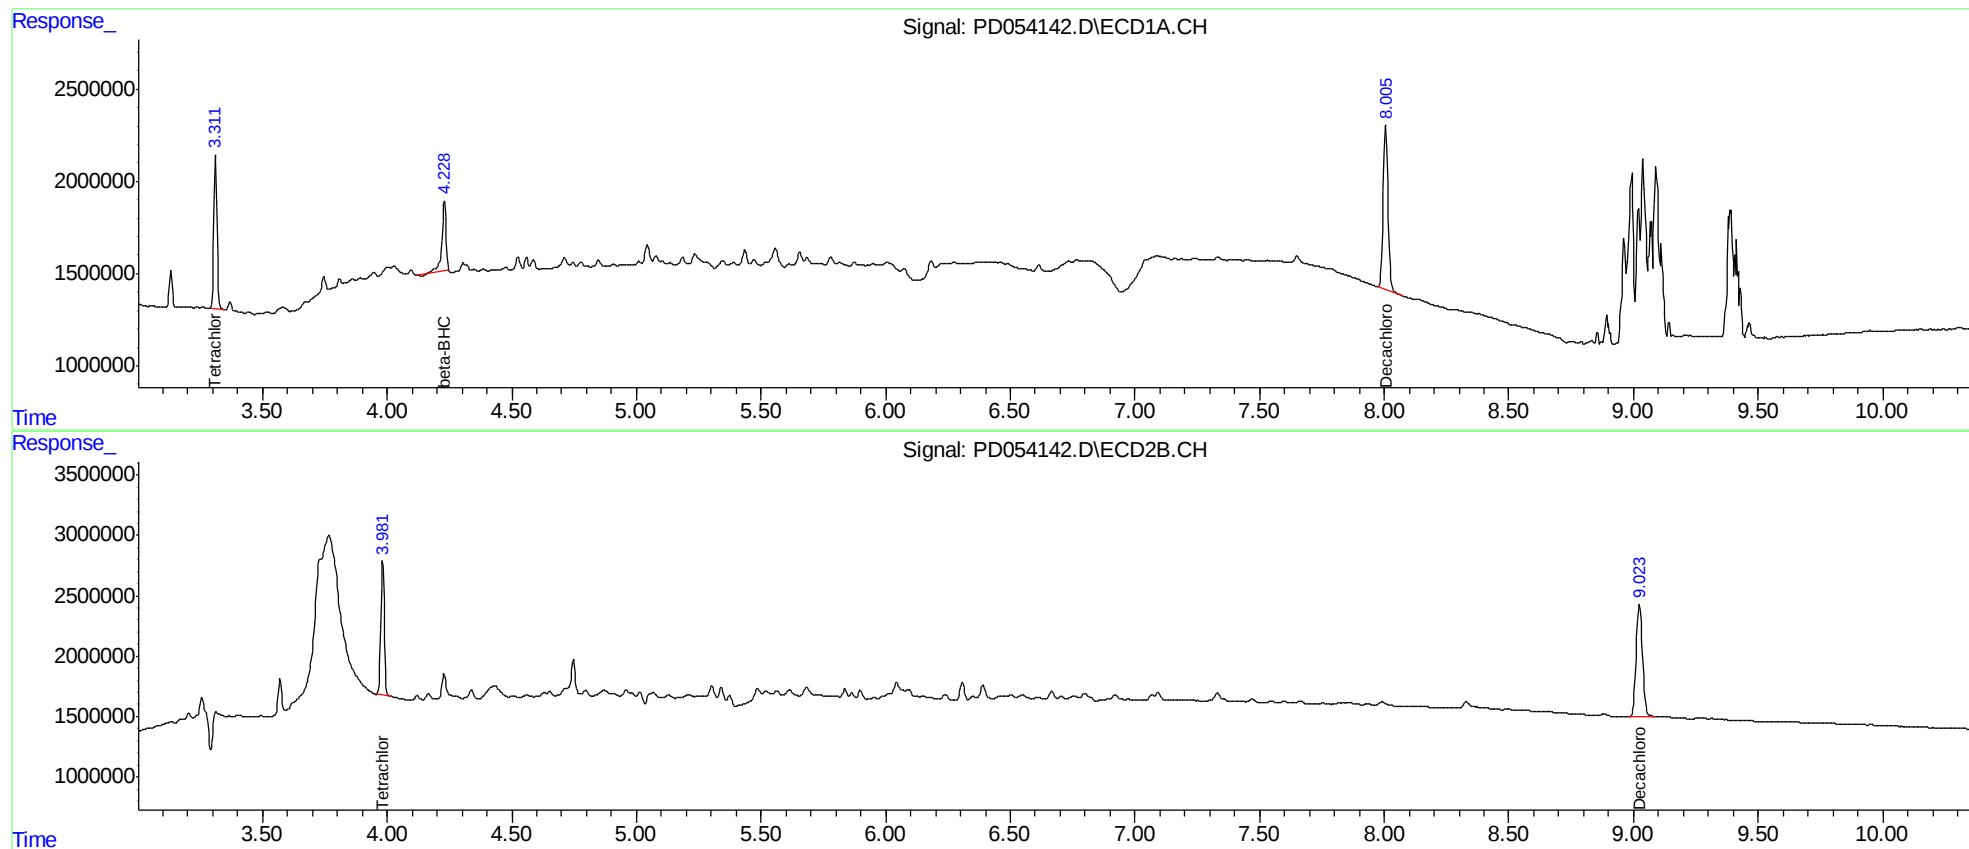


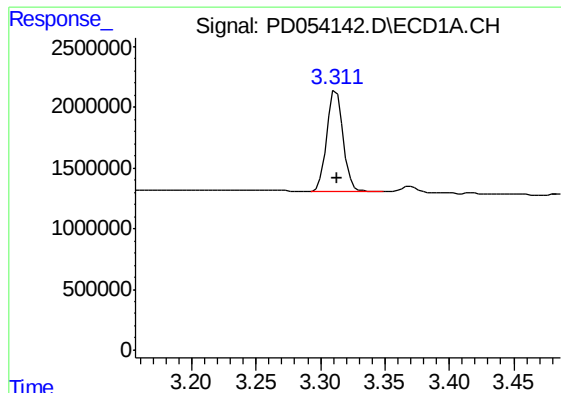

#1 Tetrachloro-m-xylene


R.T.: 3.312 min
Delta R.T.: 0.000 min
Response: 7412234
Conc: 12.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
BEP28

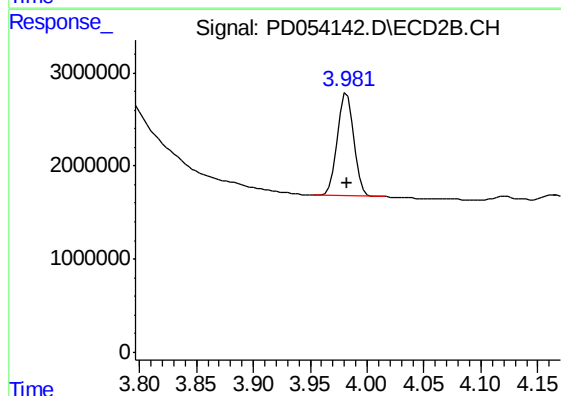


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 10979206
Conc: 11.98 ng/ml

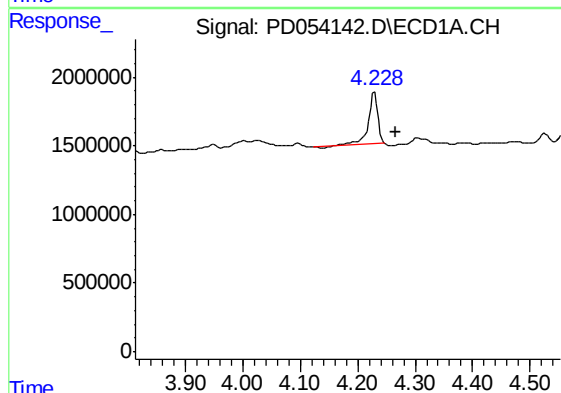


#6 beta-BHC

R.T.: 4.230 min
Delta R.T.: -0.037 min
Response: 4250409
Conc: 10.74 ng/ml

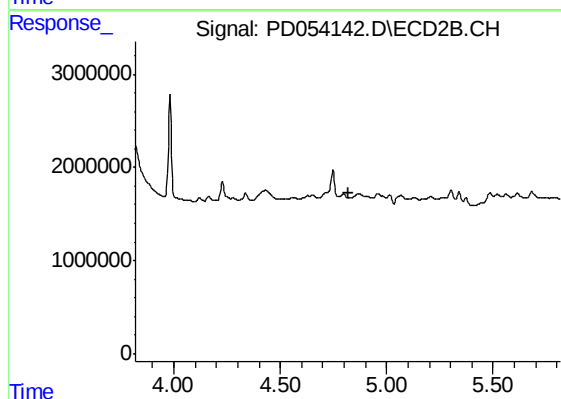

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.819 min
Response: 0
Conc: N.D.

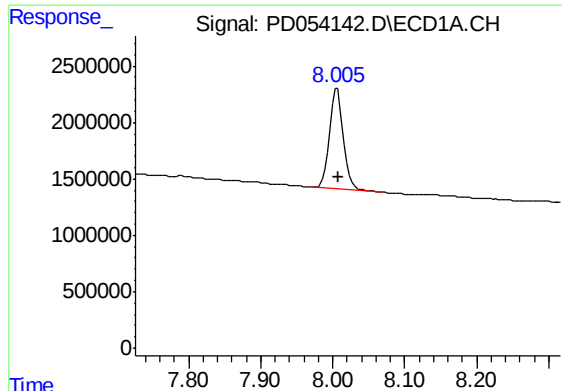

#27 Decachlorobiphenyl

R.T.: 8.006 min
Delta R.T.: -0.002 min
Response: 11877483
Conc: 16.96 ng/ml

Instrument :
ECD_D
ClientSampleId :
BEP28

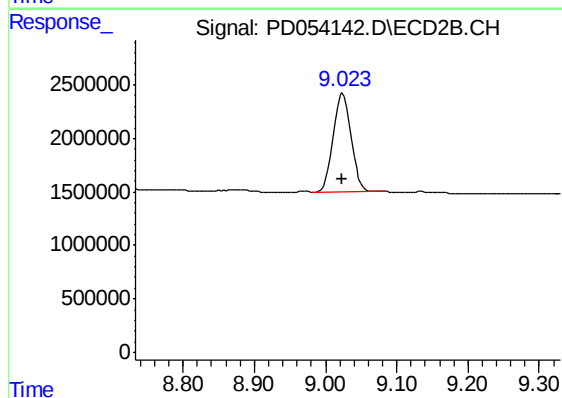

#27 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: 0.000 min
Response: 16104607
Conc: 17.15 ng/ml