

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073019\
 Data File : PD054122.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Jul 2019 13:21
 Operator : SM\AJ
 Sample : K3976-10
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0CA1

Manual Integrations
 APPROVED

Ankita
 8/1/2019 10:56:38 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 02:35:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071819CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 07:29:30 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.312	3.983	14185060	21591397	23.060	23.560
2)	SA Decachlor...	8.006	9.023	23980518	32243053	34.246	34.344
Target Compounds							
13)	MA Dieldrin	5.557	6.456	668009	933672	0.760m	0.709m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073019\
Data File : PD054122.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Jul 2019 13:21
Operator : SM\AJ
Sample : K3976-10
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 02:35:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071819CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 07:29:30 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

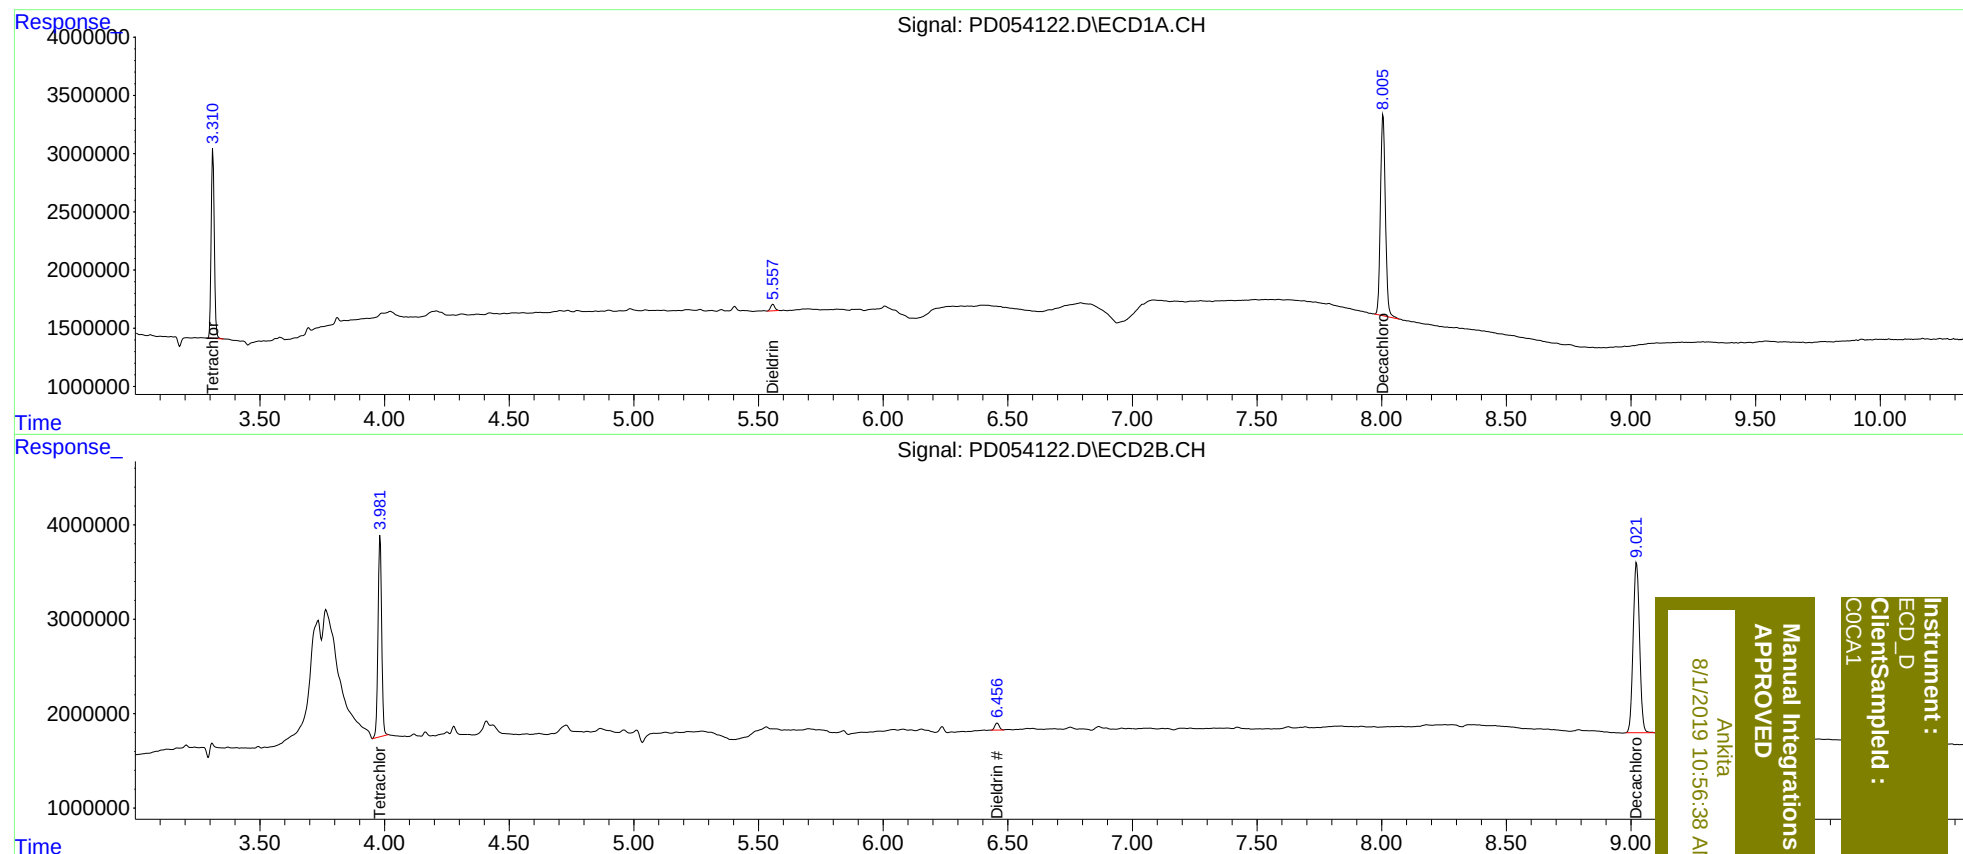

8/1/2019 10:56:38 AM

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
C0CA1