

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073019\
 Data File : PD054147.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Jul 2019 19:22
 Operator : SM\AJ
 Sample : K3935-07
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BEP29

Manual Integrations
 APPROVED

Ankita
 8/1/2019 10:57:04 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 09:58:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071819CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 07:29:30 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.312	3.982	7872588	11927533	12.798	13.015
2) SA Decachlor...	8.006	9.024	10907679	14181968	15.577	15.106
Target Compounds						
7) B delta-BHC	4.475	5.047	2993050	13726512	3.348	10.037m#
12) B 4,4'-DDE	5.432	6.307	430244	7875836	0.488m	5.919 #
14) MA Endrin	5.811	6.667	1327407	12323935	1.769m	11.932 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073019\
Data File : PD054147.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Jul 2019 19:22
Operator : SM\AJ
Sample : K3935-07
Misc :
ALS Vial : 36 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 09:58:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071819CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 07:29:30 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

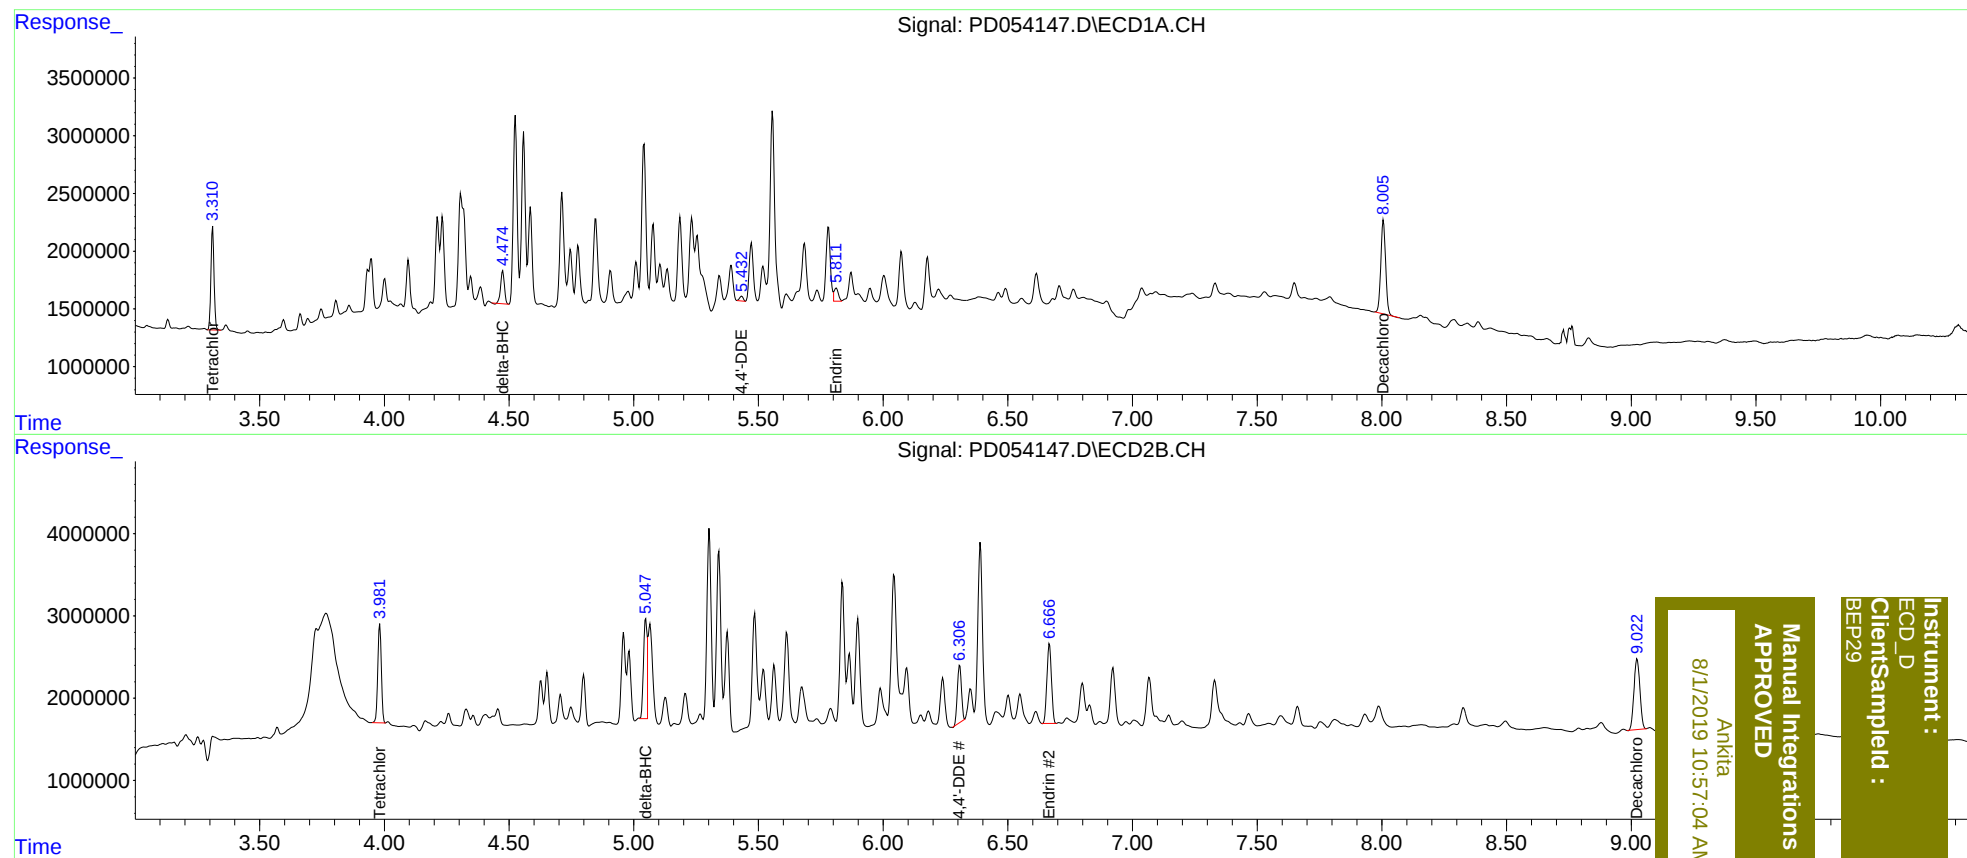

8/1/2019 10:57:04 AM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
ClientSampled :
BEP29