

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073021\
 Data File : PD064618.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2021 06:23
 Operator : AR\AJ
 Sample : M3123-07MS
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0069MS

Manual Integrations
 APPROVED

mohammad
 8/2/2021 12:38:09 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 05:16:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 28 07:07:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	5.413	4.617	42545575	163.7E6	35.666m	17.914m#
27)	SA Decachlor...	11.304	10.363	31519912	136.1E6	23.944m	22.886
Target Compounds							
2)	A alpha-BHC	5.988	5.321	100.7E6	705.5E6	61.825	57.241
3)	MA gamma-BHC...	6.385	5.741	88571328	647.8E6	56.474	56.805
4)	MA Heptachlor	7.033	6.149	91440225	603.2E6	54.409m	53.199m
5)	MB Aldrin	7.404	6.473	78687676	569.0E6	49.955	54.090
6)	B beta-BHC	6.643	6.116	39606572	278.9E6	50.767	45.976m
7)	B delta-BHC	6.908	6.378	92326017	615.5E6	53.056	56.661
8)	B Heptachlo...	7.874	7.046	77889324	455.7E6	45.368	49.229
9)	A Endosulfan I	8.279	7.449	73103079	429.2E6	51.859	55.810
10)	B trans-Chl...	8.141	7.321	120.2E6	479.5E6	75.040m	52.867m#
11)	B cis-Chlor...	8.225	7.392	97711933	436.0E6	62.712	49.008
12)	B 4,4'-DDE	8.421	7.604	152.6E6	752.3E6	105.846	99.712
13)	MA Dieldrin	8.569	7.732	161.2E6	751.7E6	108.087	93.588m
14)	MA Endrin	8.807	8.024	141.1E6	580.4E6	110.229	101.029
15)	B Endosulfa...	9.043	8.333	130.0E6	553.3E6	100.122	95.856
16)	A 4,4'-DDD	8.961	8.186	156.8E6	604.6E6	127.772	104.970
17)	MA 4,4'-DDT	9.279	8.445	134.9E6	626.1E6	103.309	113.742m
18)	B Endrin al...	9.179	8.518	119.7E6	447.7E6	105.636	90.711m
19)	B Endosulfa...	9.418	8.749	159.3E6	578.9E6	115.608	107.393m
20)	A Methoxychlor	9.770	9.038	370.1E6	1268.4E6	517.266	495.349m
21)	B Endrin ke...	9.914	9.269	162.9E6	580.1E6	107.658	96.716

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073021\
Data File : PD064618.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2021 06:23
Operator : AR\AJ
Sample : M3123-07MS
Misc :
ALS Vial : 50 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 05:16:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 28 07:07:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

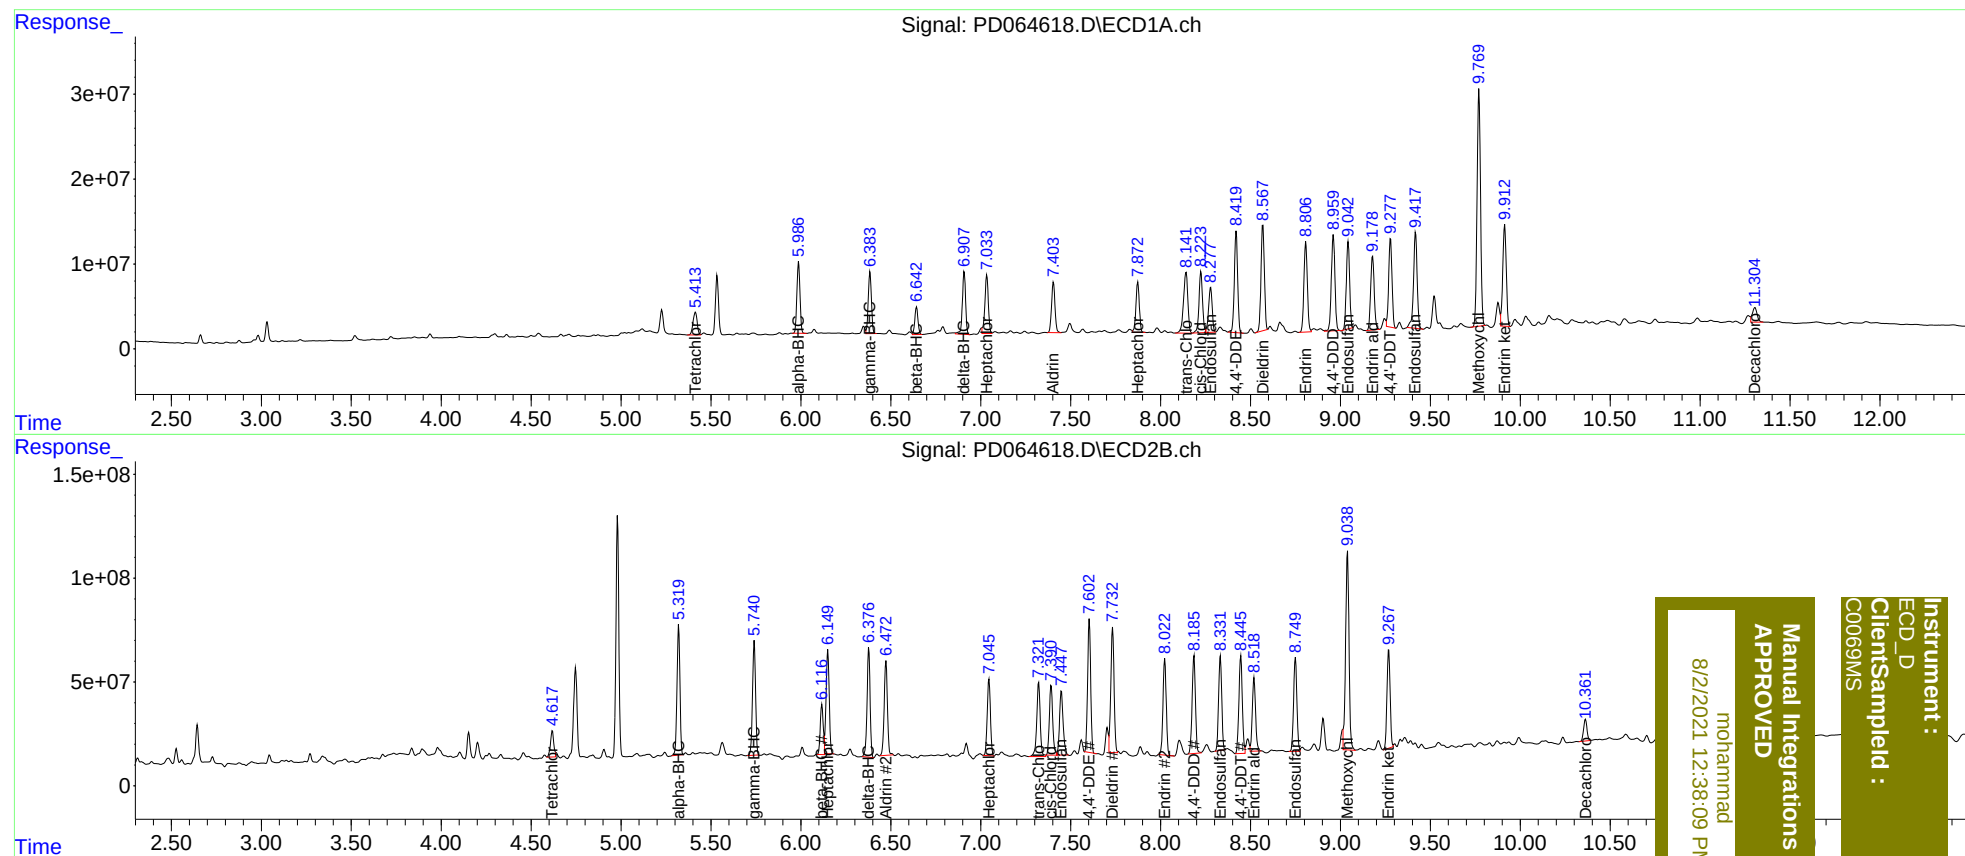

8/2/2021 12:38:09 PM
mohammad

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sample :
C0069MS