

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073021\
 Data File : PD064619.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2021 06:39
 Operator : AR\AJ
 Sample : M3123-08MSD
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0069MSD

Manual Integrations
 APPROVED

mohammad
 8/2/2021 12:38:12 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 01:13:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 28 07:07:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	5.412	4.616	42750609	159.9E6	35.838m	17.499m#
27)	SA Decachlor...	11.303	10.362	32148221	145.3E6	24.422m	24.438
Target Compounds							
2)	A alpha-BHC	5.987	5.320	99645658	691.7E6	61.166	56.118
3)	MA gamma-BHC...	6.385	5.740	87695837	639.1E6	55.916	56.043
4)	MA Heptachlor	7.033	6.148	88468086	607.4E6	52.641m	53.571m
5)	MB Aldrin	7.404	6.473	77233575	562.8E6	49.032	53.506
6)	B beta-BHC	6.643	6.115	39055875	280.0E6	50.061	46.152m
7)	B delta-BHC	6.909	6.378	91125047	608.5E6	52.366	56.010
8)	B Heptachlo...	7.874	7.046	76693529	448.8E6	44.671	48.482
9)	A Endosulfan I	8.278	7.449	72860409	428.3E6	51.687	55.705
10)	B trans-Chl...	8.140	7.322	119.7E6	483.3E6	74.711m	53.287m#
11)	B cis-Chlor...	8.224	7.392	97540439	431.7E6	62.602	48.532
12)	B 4,4'-DDE	8.420	7.604	151.2E6	749.5E6	104.901	99.331
13)	MA Dieldrin	8.568	7.732	160.2E6	750.8E6	107.420	93.475m
14)	MA Endrin	8.807	8.024	139.9E6	579.8E6	109.248	100.924
15)	B Endosulfa...	9.042	8.332	127.5E6	549.8E6	98.152	95.246
16)	A 4,4'-DDD	8.960	8.186	155.5E6	596.4E6	126.660	103.552
17)	MA 4,4'-DDT	9.277	8.445	138.7E6	625.7E6	106.258m	113.665m
18)	B Endrin al...	9.178	8.519	121.4E6	451.8E6	107.130	91.548m
19)	B Endosulfa...	9.417	8.750	157.4E6	547.5E6	114.243	101.580
20)	A Methoxychlor	9.770	9.038	366.1E6	1262.5E6	511.602	493.067m
21)	B Endrin ke...	9.913	9.269	162.0E6	575.6E6	107.071	95.961

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073021\
Data File : PD064619.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2021 06:39
Operator : AR\AJ
Sample : M3123-08MSD
Misc :
ALS Vial : 51 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 01:13:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 28 07:07:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

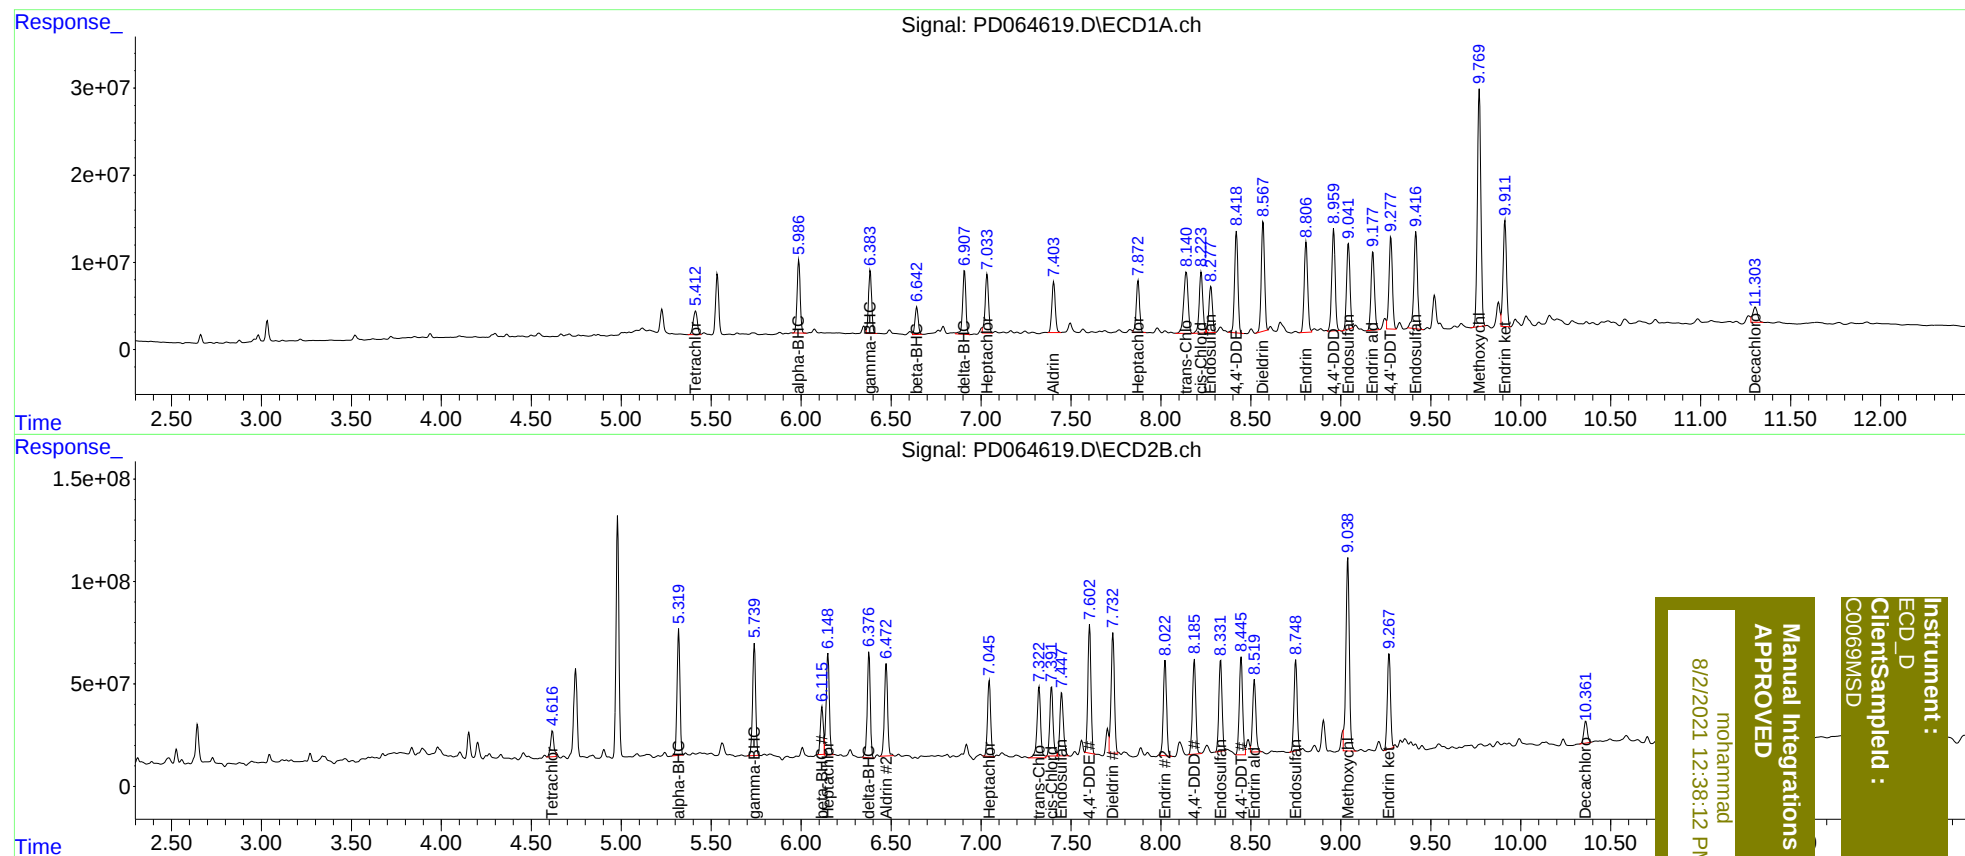

8/2/2021 12:38:12 PM
mohammad

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
C0069MSD