

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073021\
 Data File : PD064556.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jul 2021 13:01
 Operator : AR\AJ
 Sample : M3091-11
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0049

Manual Integrations
 APPROVED

mohammad
 8/2/2021 12:35:57 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 02:45:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 28 07:07:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	5.405	4.617	17283073	146.5E6	14.488	16.037m
27)	SA Decachlor...	11.304	10.362	29589565	152.2E6	22.478	25.591
Target Compounds							
3)	MA gamma-BHC...	6.393	5.734	1310879	36328761	0.836	3.186 #
10)	B trans-Chl...	8.123	7.304	73916886	338.4E6	46.127m	37.314m
13)	MA Dieldrin	8.570	7.741	75268542	189.3E6	50.472m	23.573 #
14)	MA Endrin	8.812	8.038	26609518	214.9E6	20.782	37.406 #
15)	B Endosulfa...	9.028	8.331	34391071	96264650	26.483	16.677 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073021\
Data File : PD064556.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jul 2021 13:01
Operator : AR\AJ
Sample : M3091-11
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 02:45:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 28 07:07:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

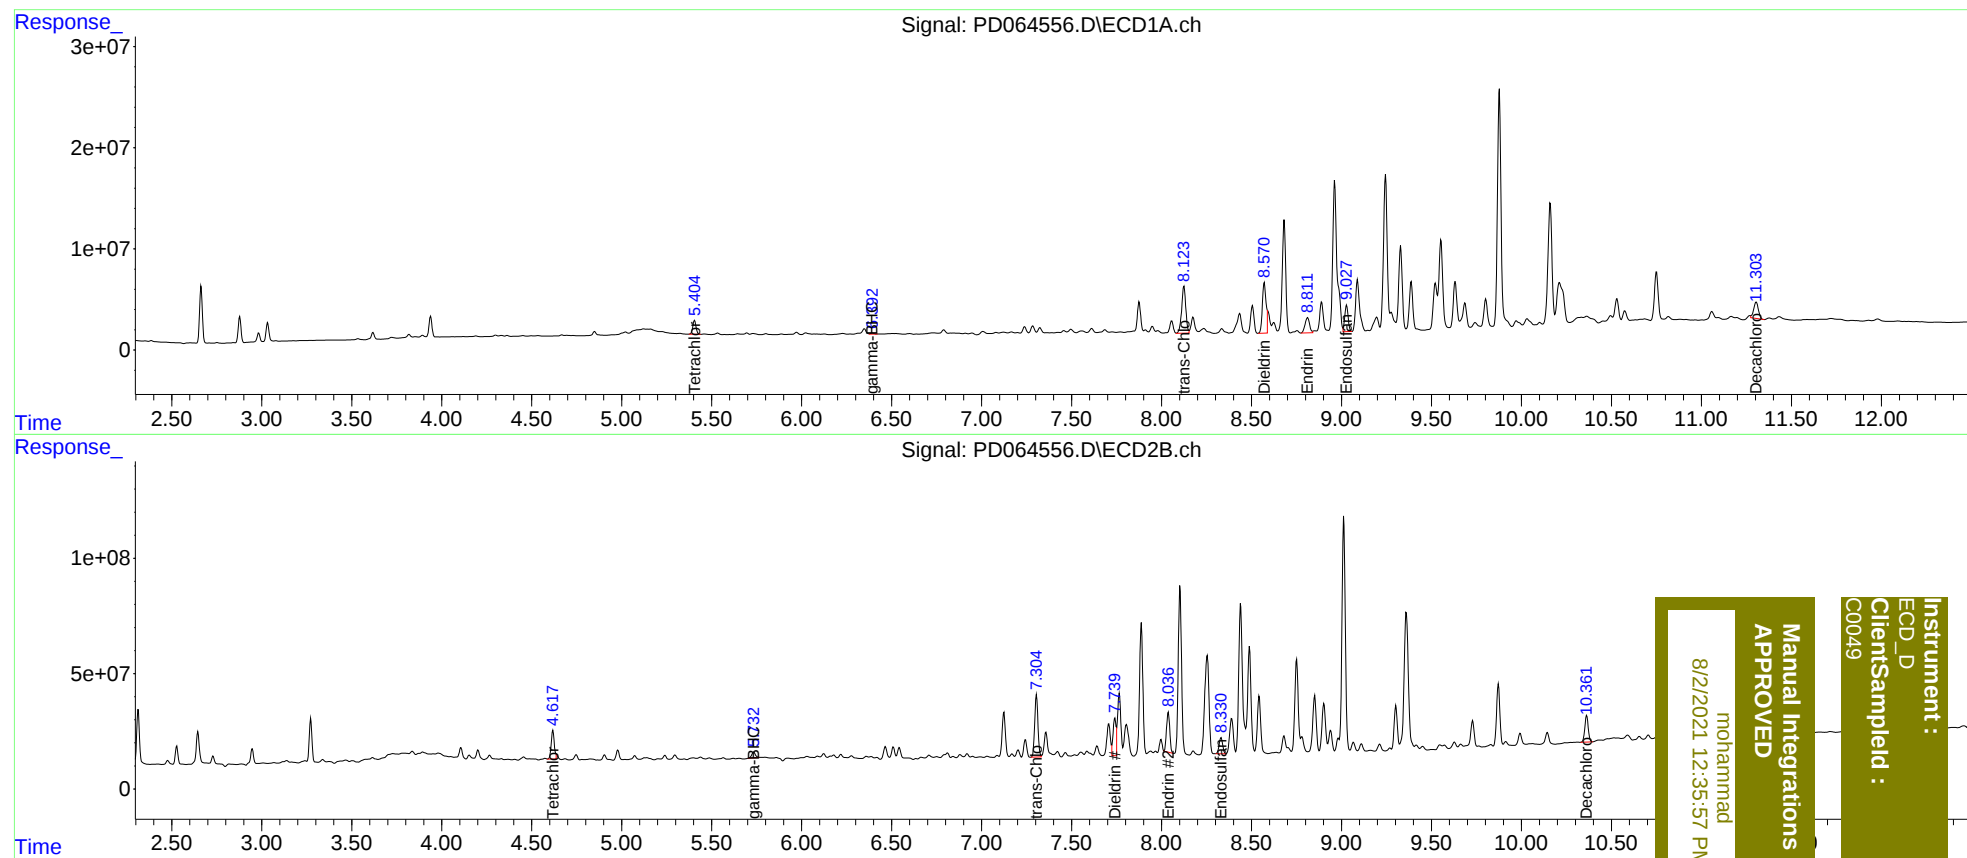

8/2/2021 12:35:57 PM

Manual Integrations
APPROVED

mohammad

Instrument :
ECD_D
ClientSampled :
C0049