

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073021\
 Data File : PD064571.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jul 2021 17:23
 Operator : AR\AJ
 Sample : M3106-09
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGD20

Manual Integrations
 APPROVED

mohammad
 8/2/2021 12:36:35 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 03:56:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 28 07:07:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	5.405	4.618	14044391	122.0E6	11.773	13.356
27)	SA Decachlor...	11.304	10.364	24306640	102.6E6	18.465m	17.253
Target Compounds							
10)	B trans-Chl...	8.129	7.304	9154722	30681771	5.713m	3.383m#
11)	B cis-Chlor...	8.228	7.386	2476357	15422601	1.589	1.734m
12)	B 4,4'-DDE	8.419	7.603	3294446	13810029	2.286	1.830
14)	MA Endrin	8.814	8.037	4572027	7009960	3.571	1.220m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073021\
Data File : PD064571.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jul 2021 17:23
Operator : AR\AJ
Sample : M3106-09
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 03:56:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 28 07:07:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

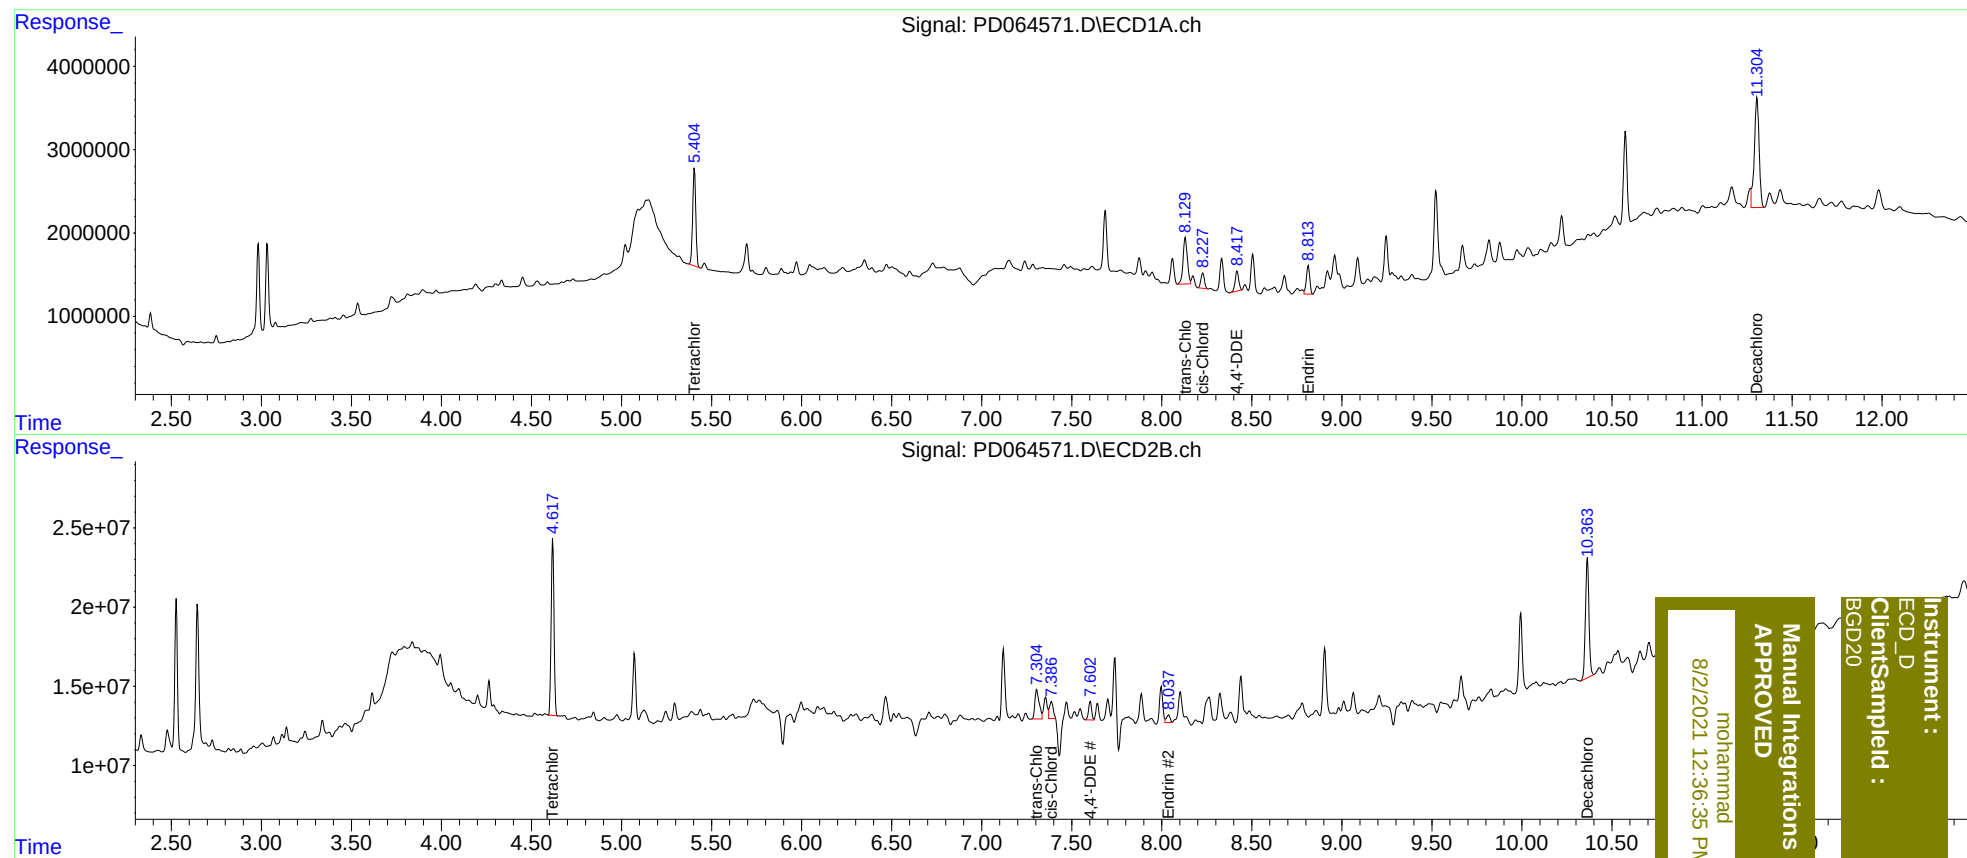

8/2/2021 12:36:35 PM

Manual Integrations
APPROVED

mohammad

Instrument :
ECD_D
ClientSampled :
BGD20