

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073022\
 Data File : PD071229.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jul 2022 15:55
 Operator : AR\AJ
 Sample : PB146542BS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS542

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/29/2022
 Supervised By :Ankita Jodhani 07/29/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 04:51:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071322CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 13 15:03:36 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.480	4.125	42764175	483.3E6	18.379	21.420
27)	SA Decachlor...	8.250	9.326	81714333	324.0E6	34.015	36.594
Target Compounds							
2)	A alpha-BHC	3.921	4.528	20449564	166.9E6	5.792	5.399m
3)	MA gamma-BHC...	4.206	4.824	18300895	147.8E6	5.416	5.802
4)	MA Heptachlor	4.505	5.340	15235185	109.0E6	4.471	5.527
5)	MB Aldrin	4.754	5.653	15652875	93755775	4.447	5.546
6)	B beta-BHC	4.454	4.999	6953457	55263975	4.682m	4.581m
7)	B delta-BHC	4.660	5.224	12202662	108.6E6	3.610m	4.951m#
8)	B Heptachlo...	5.199	6.049	14672070	78284961	4.582	5.500
9)	A Endosulfan I	5.539	6.414	13641654	72296698	4.710	5.711
10)	B trans-Chl...	5.426	6.286	15126806	76993311	4.564	5.374
11)	B cis-Chlor...	5.485	6.359	14536246	75489026	4.500	5.442
12)	B 4,4'-DDE	5.651	6.514	26721422	147.3E6	8.600	11.194 #
13)	MA Dieldrin	5.784	6.675	29874050	156.4E6	9.167	11.846 #
14)	MA Endrin	6.042	6.897	24538122	107.9E6	9.131	10.588m
15)	B Endosulfa...	6.316	7.113	25498770	134.9E6	9.652	12.373 #
16)	A 4,4'-DDD	6.169	7.014	22795367	111.9E6	9.149	10.310
17)	MA 4,4'-DDT	6.410	7.316	23264676	127.1E6	8.840	11.669 #
18)	B Endrin al...	6.486	7.239	20114607	99699279	8.970	10.778
19)	B Endosulfa...	6.699	7.463	23752107	113.3E6	8.961	10.531
20)	A Methoxychlor	6.961	7.775	67996658	299.4E6	51.280	59.869
21)	B Endrin ke...	7.193	7.945	30472675	157.6E6	10.342	13.476 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073022\
Data File : PD071229.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jul 2022 15:55
Operator : AR\AJ
Sample : PB146542BS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 04:51:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071322CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 13 15:03:36 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

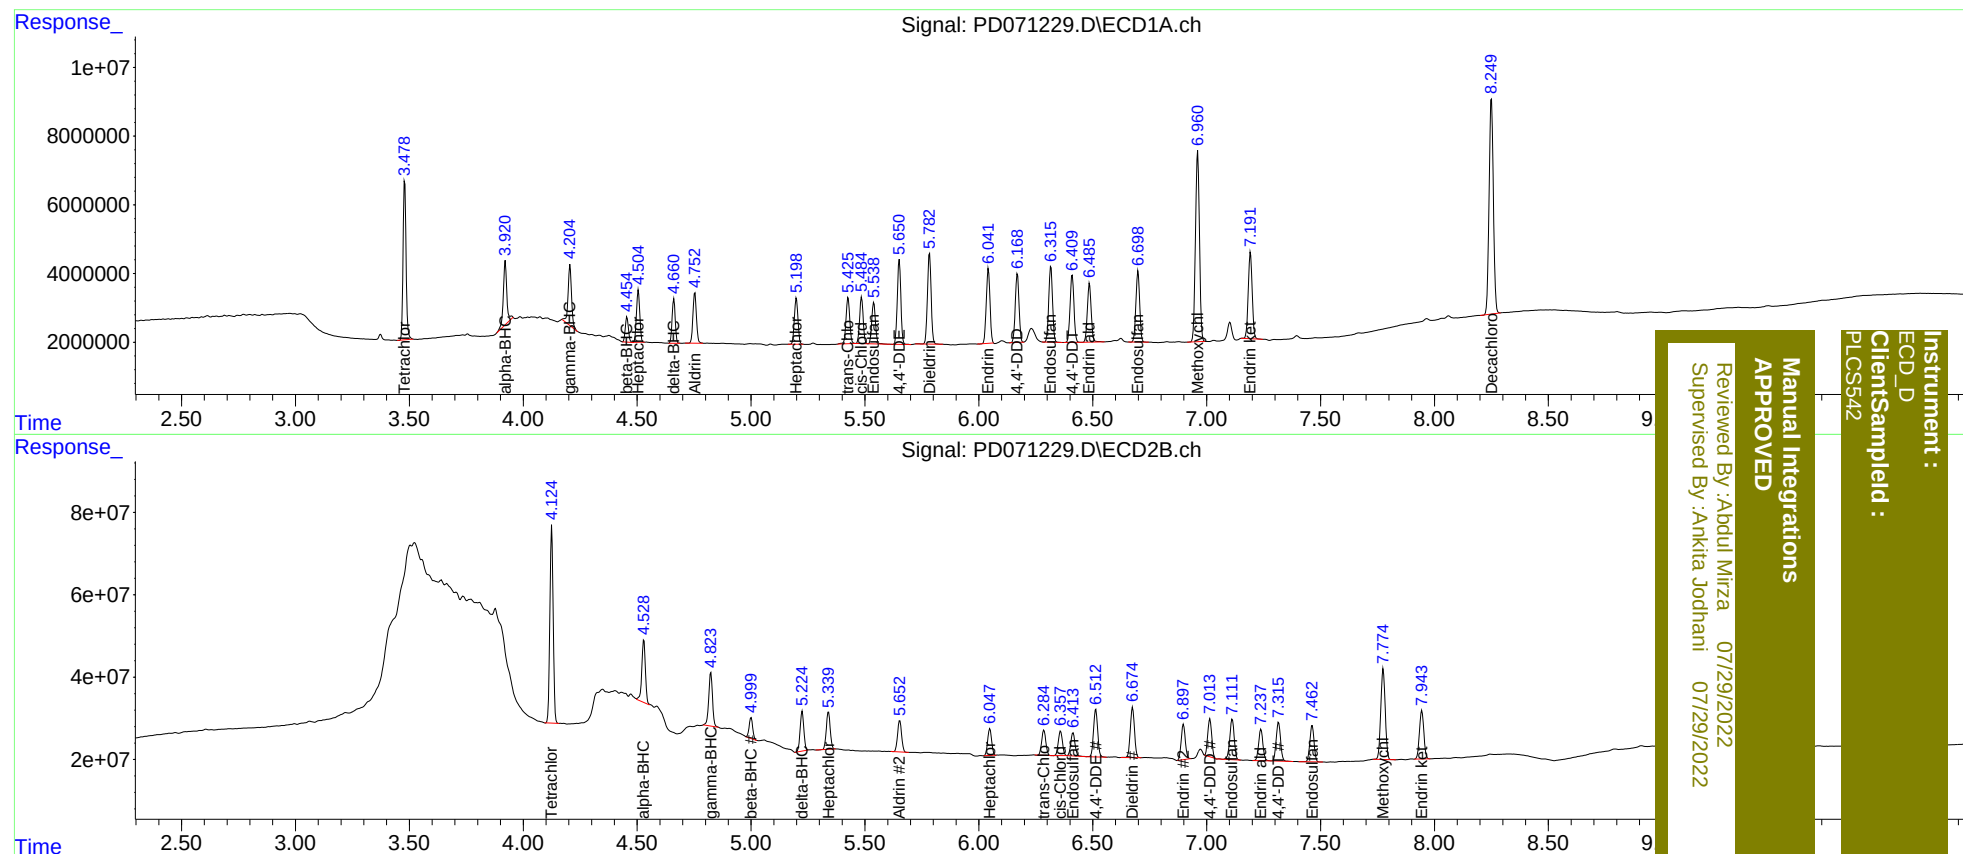

Reviewed By: Abdul Mirza 07/29/2022
Supervised By: Ankita Jodhani 07/29/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client/Sampled :
PLCS542