

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073118\
 Data File : PD048657.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Jul 2018 20:05
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 10:57:11 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX073118.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 01 10:17:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	3.371	3.968	22280603	281.4E6	19.297	19.935
7) SA Decachlor...	8.067	8.994	29194947	340.7E6	20.365	20.761

Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073118\
Data File : PD048657.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Jul 2018 20:05
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 10:57:11 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX073118.M
Quant Title : GC Extractables
QLast Update : Wed Aug 01 10:17:31 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

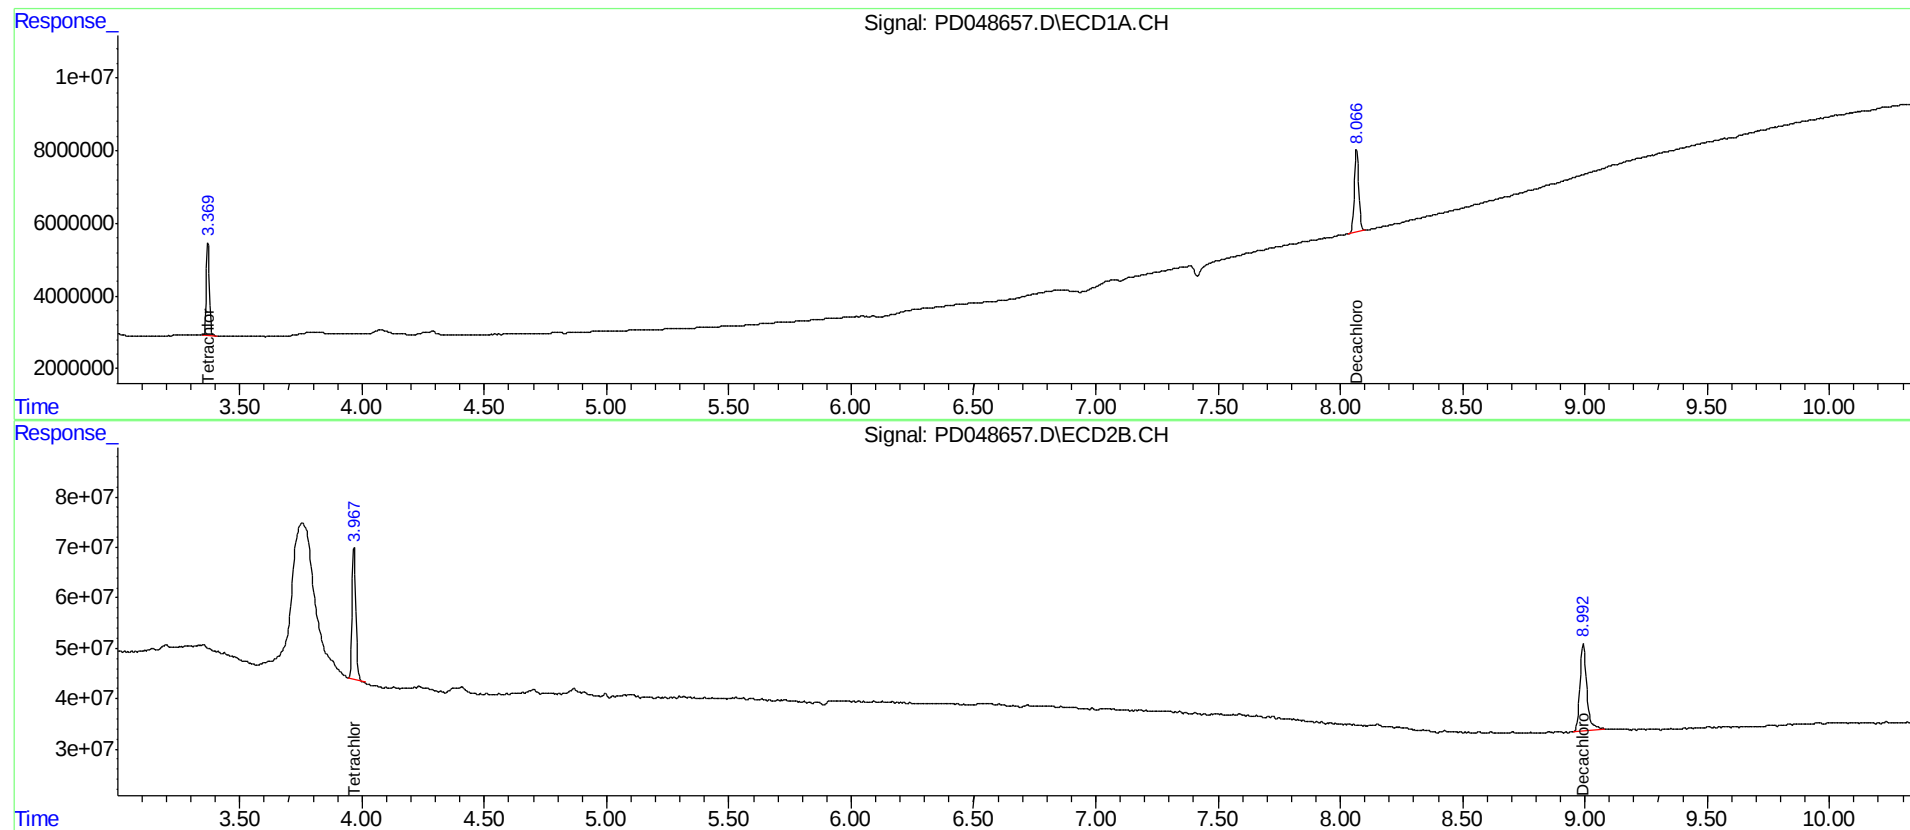


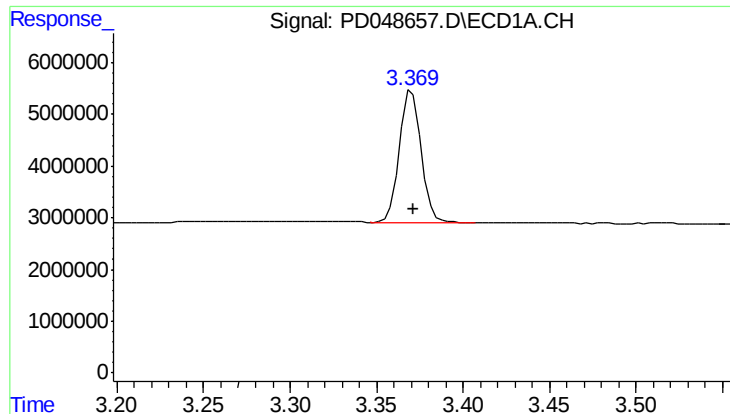

#1 Tetrachloro-m-xylene


R.T.: 3.371 min
Delta R.T.: 0.000 min
Response: 22280603
Conc: 19.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

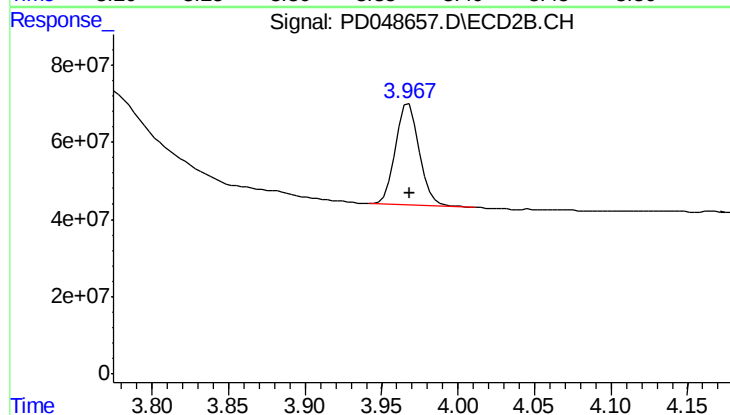


#1 Tetrachloro-m-xylene

R.T.: 3.968 min
Delta R.T.: 0.000 min
Response: 281386310
Conc: 19.94 ng/ml

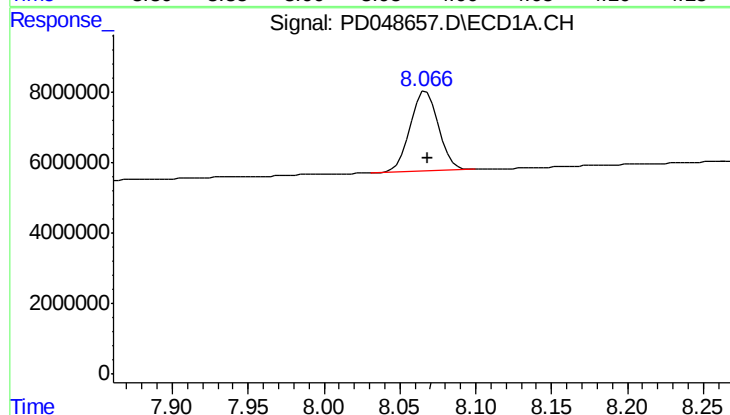

#7 Decachlorobiphenyl

R.T.: 8.067 min
Delta R.T.: 0.000 min
Response: 29194947
Conc: 20.37 ng/ml

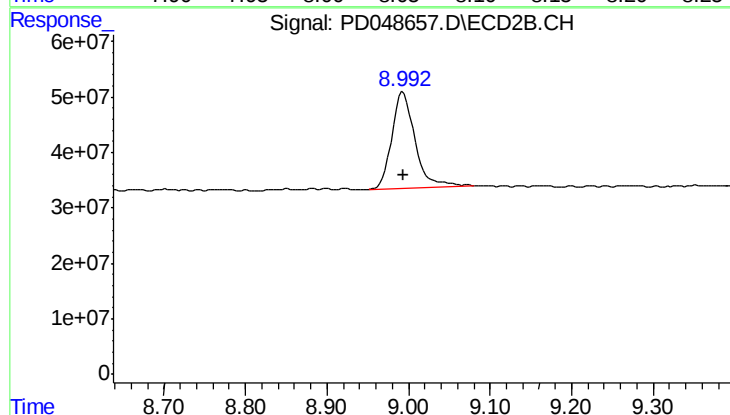

#7 Decachlorobiphenyl

R.T.: 8.994 min
Delta R.T.: 0.000 min
Response: 340662421
Conc: 20.76 ng/ml