

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073125\
 Data File : PD089695.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2025 13:23
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 06:19:33 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 01 06:17:51 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.877	120.5E6	945.6E6	50.000	50.000
28)	SA Decachlor...	9.069	8.067	176.9E6	974.5E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.712	3.902	84493998	372.7E6	500.000	500.000
24)	Chlordane-2	5.238	4.483	85139038	388.8E6	500.000	500.000
25)	Chlordane-3	5.944	5.122	351.5E6	1170.3E6	500.000	500.000
26)	Chlordane-4	6.029	5.186	426.3E6	1005.1E6	500.000	500.000
27)	Chlordane-5	6.868	6.086	72983349	462.5E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073125\
Data File : PD089695.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2025 13:23
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 06:19:33 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
Quant Title : GC Extractables
QLast Update : Fri Aug 01 06:17:51 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

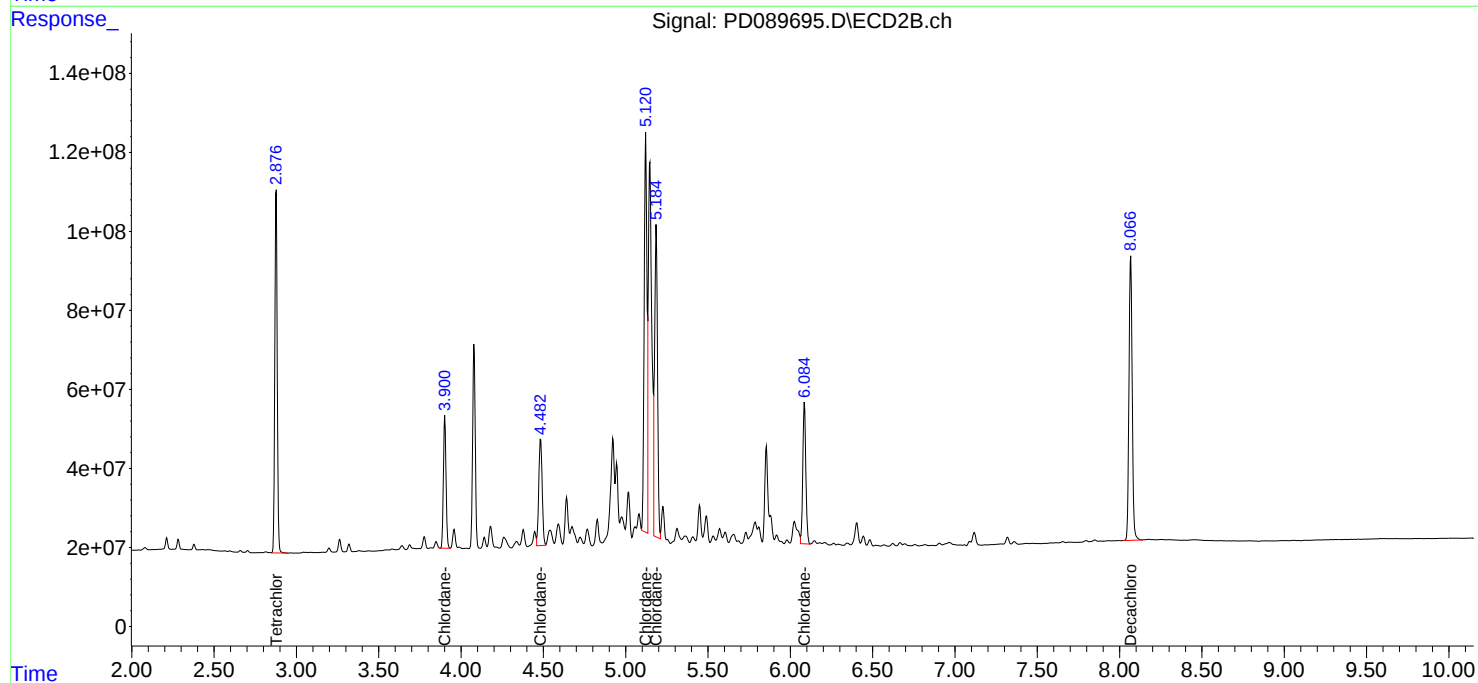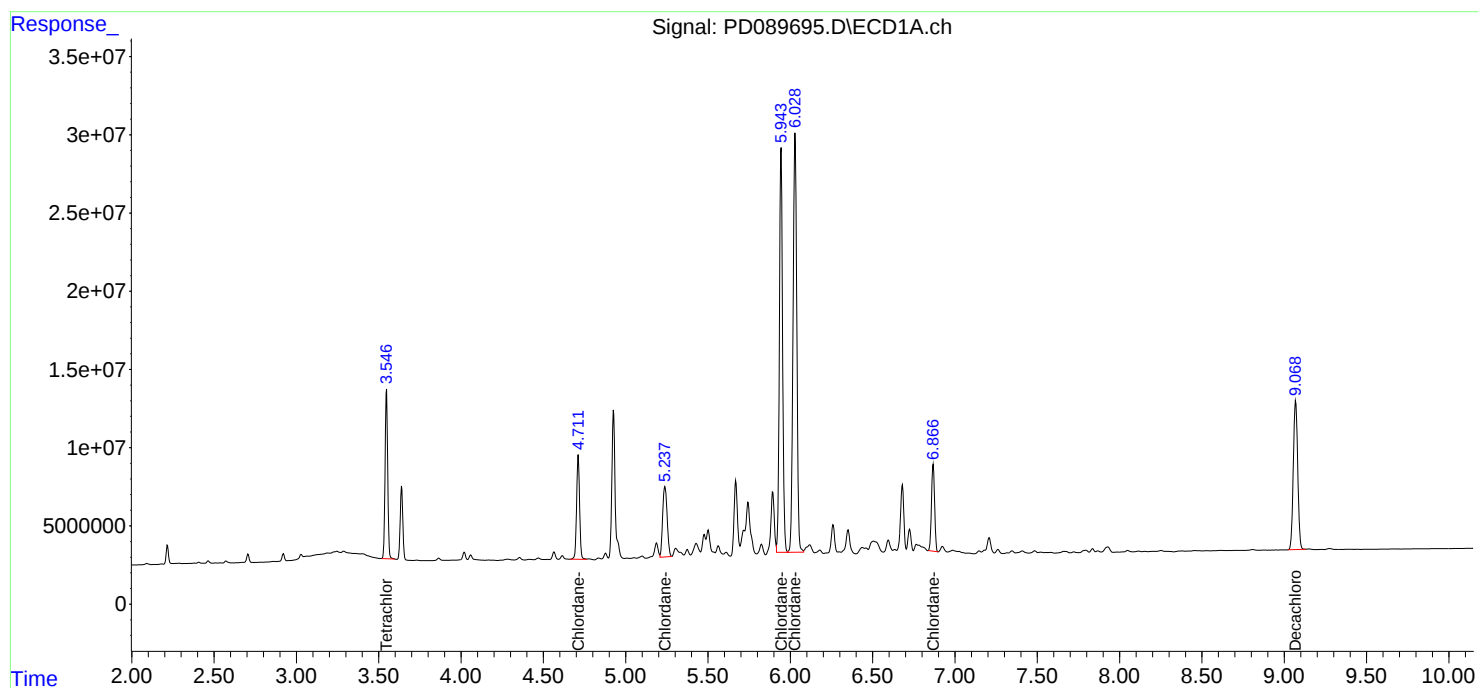


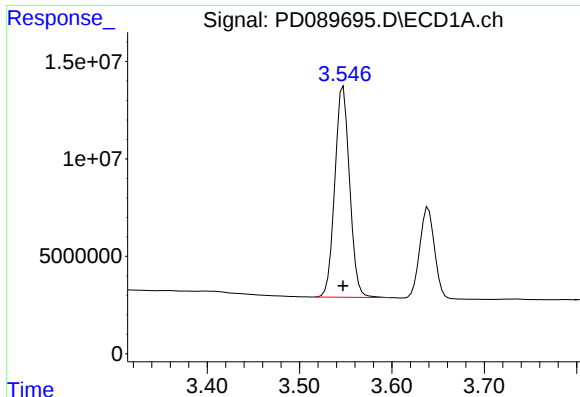

#1 Tetrachloro-m-xylene


R.T.: 3.547 min
Delta R.T.: 0.000 min
Response: 120454144
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

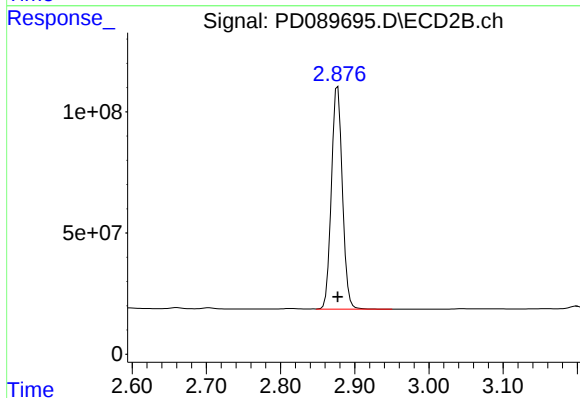


#1 Tetrachloro-m-xylene

R.T.: 2.877 min
Delta R.T.: 0.000 min
Response: 945590516
Conc: 50.00 ng/ml

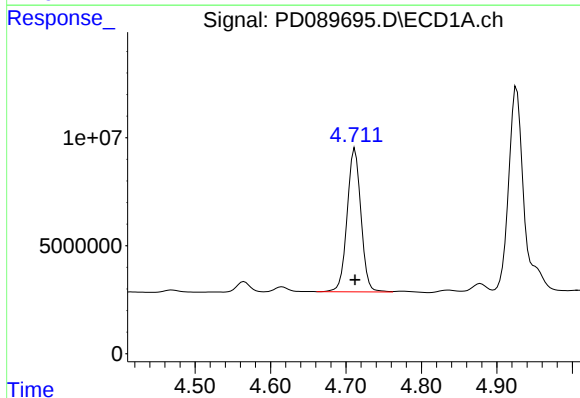


#23 Chlordane-1

R.T.: 4.712 min
Delta R.T.: 0.000 min
Response: 84493998
Conc: 500.00 ng/ml

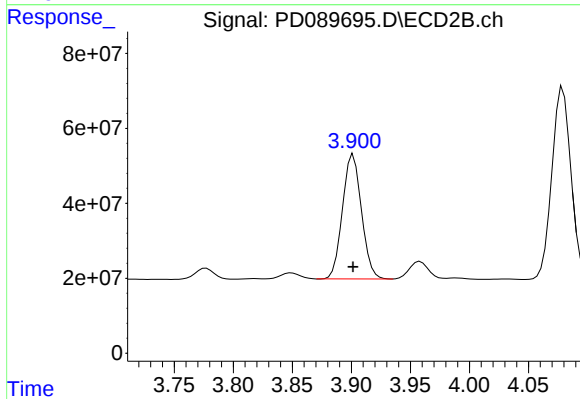

#23 Chlordane-1


R.T.: 3.902 min
Delta R.T.: 0.000 min
Response: 372667142
Conc: 500.00 ng/ml

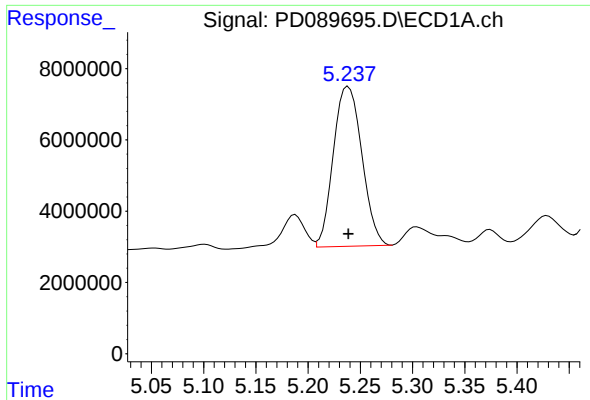

#24 Chlordane-2


R.T.: 5.238 min
Delta R.T.: 0.000 min
Response: 85139038
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

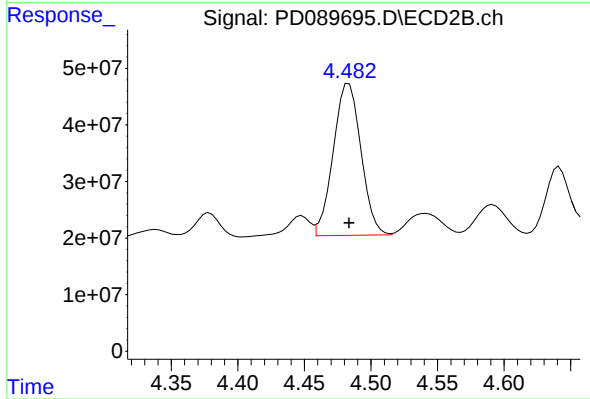


#24 Chlordane-2

R.T.: 4.483 min
Delta R.T.: 0.000 min
Response: 388836209
Conc: 500.00 ng/ml

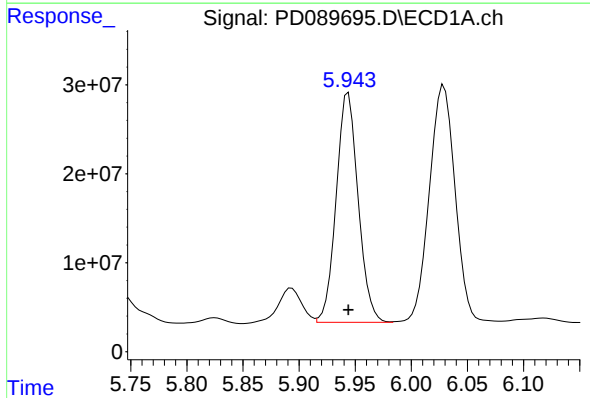


#25 Chlordane-3

R.T.: 5.944 min
Delta R.T.: 0.000 min
Response: 351491901
Conc: 500.00 ng/ml

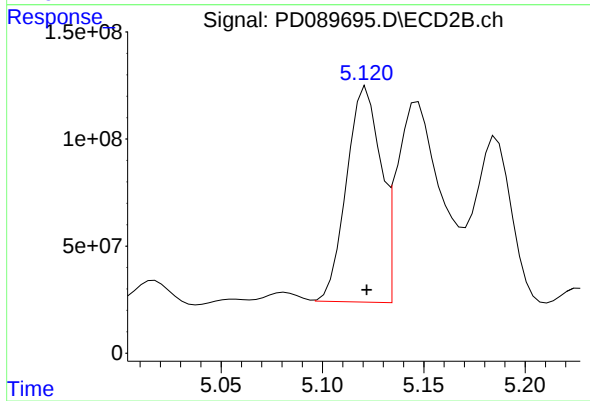

#25 Chlordane-3


R.T.: 5.122 min
Delta R.T.: 0.000 min
Response: 1170269551
Conc: 500.00 ng/ml

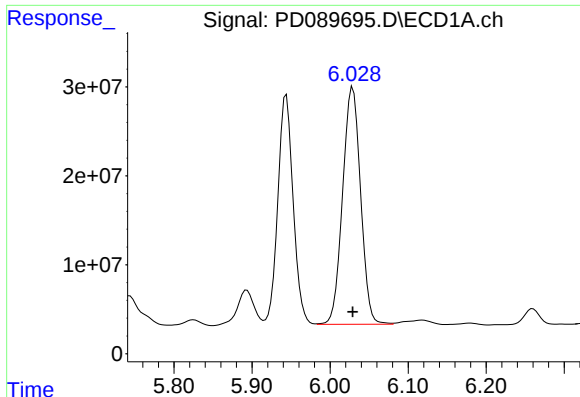

#26 Chlordane-4


R.T.: 6.029 min
Delta R.T.: 0.000 min
Response: 426332129
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

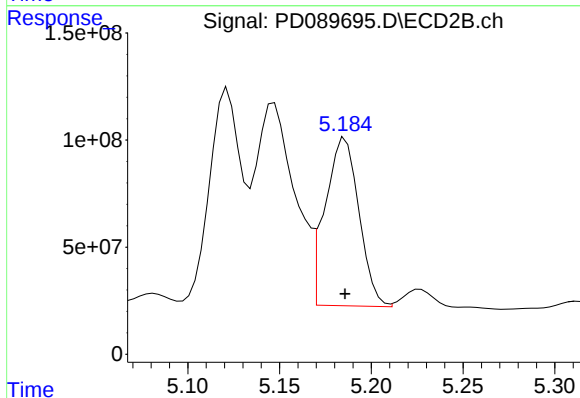


#26 Chlordane-4

R.T.: 5.186 min
Delta R.T.: 0.000 min
Response: 1005074647
Conc: 500.00 ng/ml

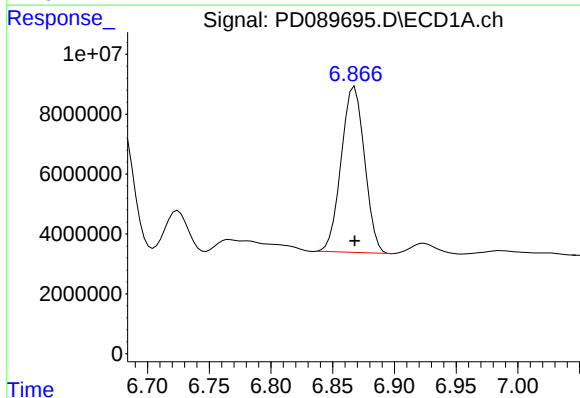


#27 Chlordane-5

R.T.: 6.868 min
Delta R.T.: 0.000 min
Response: 72983349
Conc: 500.00 ng/ml

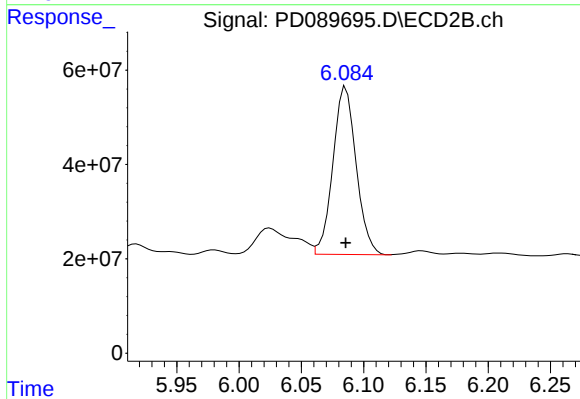

#27 Chlordane-5


R.T.: 6.086 min
Delta R.T.: 0.000 min
Response: 462521233
Conc: 500.00 ng/ml

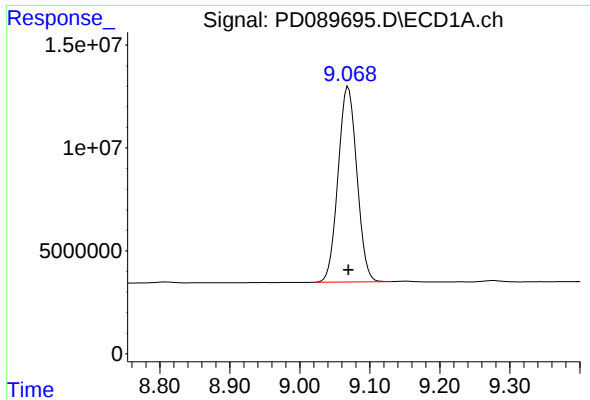

#28 Decachlorobiphenyl

R.T.: 9.069 min
Delta R.T.: 0.000 min
Response: 176909463
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

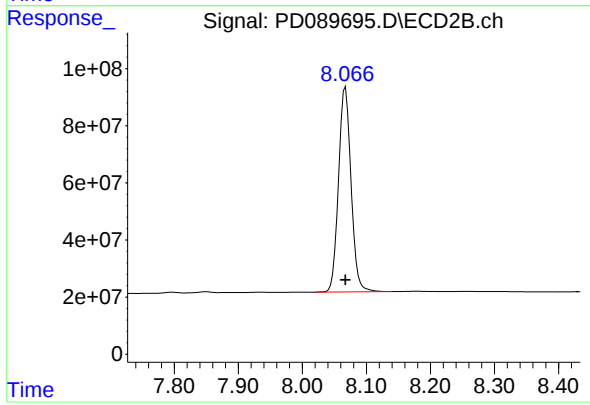

#28 Decachlorobiphenyl

R.T.: 8.067 min
Delta R.T.: 0.000 min
Response: 974452764
Conc: 50.00 ng/ml