

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080118\
Data File : PD048674.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Aug 2018 11:04
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 11:55:23 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX073118.M
Quant Title : GC Extractables
QLast Update : Wed Aug 01 10:17:31 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	3.371	3.968	22748860	295.1E6	19.702	20.907
7) SA Decachlor...	8.068	8.993	29279176	356.4E6	20.424	21.723

Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080118\
Data File : PD048674.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Aug 2018 11:04
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 11:55:23 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX073118.M
Quant Title : GC Extractables
QLast Update : Wed Aug 01 10:17:31 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

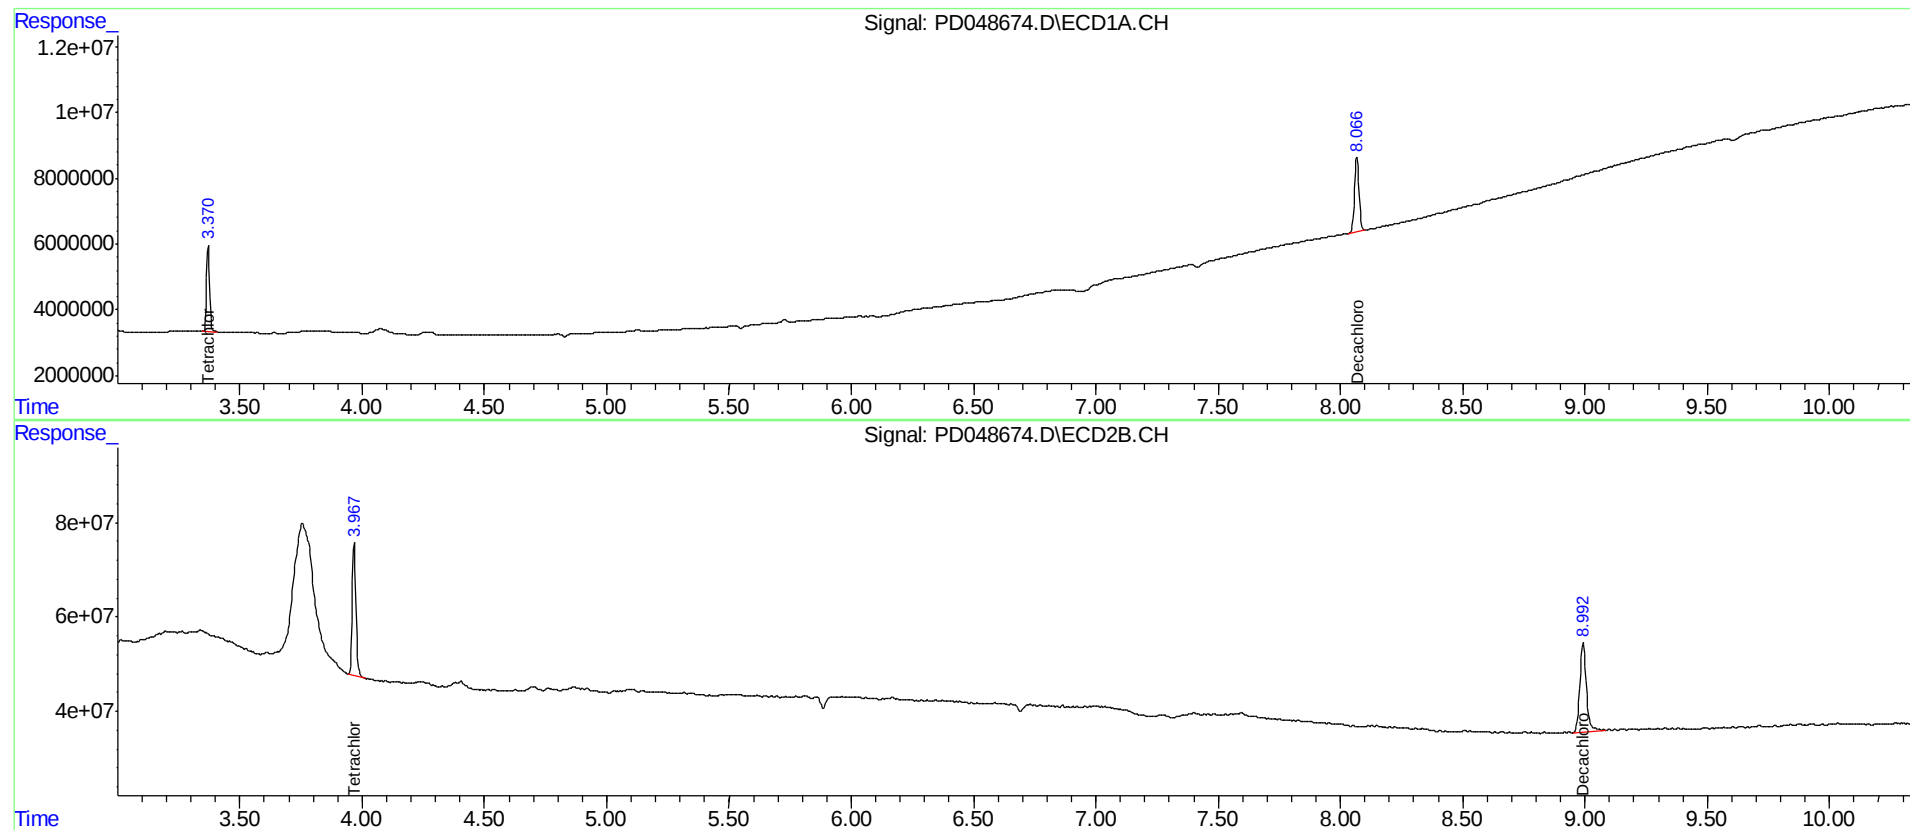


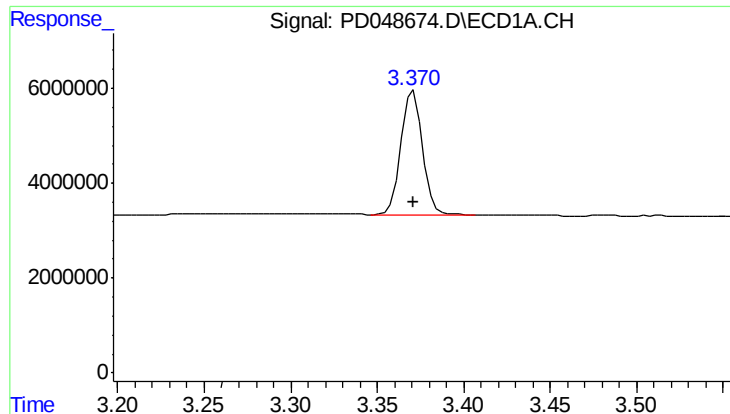

#1 Tetrachloro-m-xylene


R.T.: 3.371 min
Delta R.T.: 0.000 min
Response: 22748860
Conc: 19.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

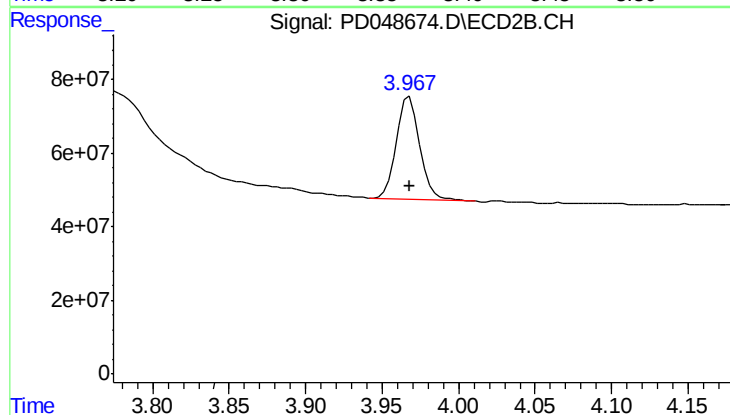


#1 Tetrachloro-m-xylene

R.T.: 3.968 min
Delta R.T.: 0.000 min
Response: 295094754
Conc: 20.91 ng/ml

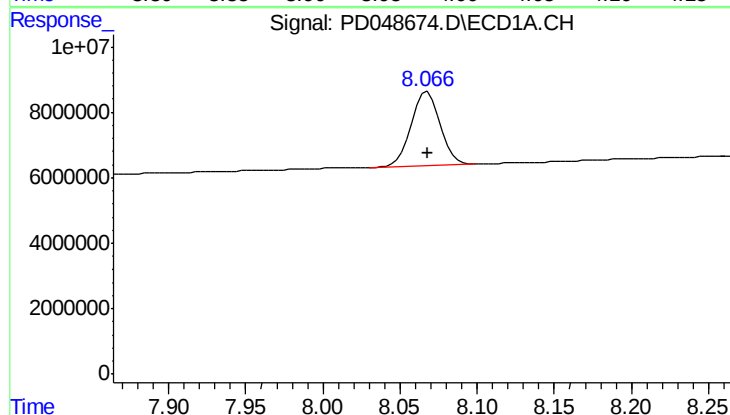

#7 Decachlorobiphenyl

R.T.: 8.068 min
Delta R.T.: 0.000 min
Response: 29279176
Conc: 20.42 ng/ml

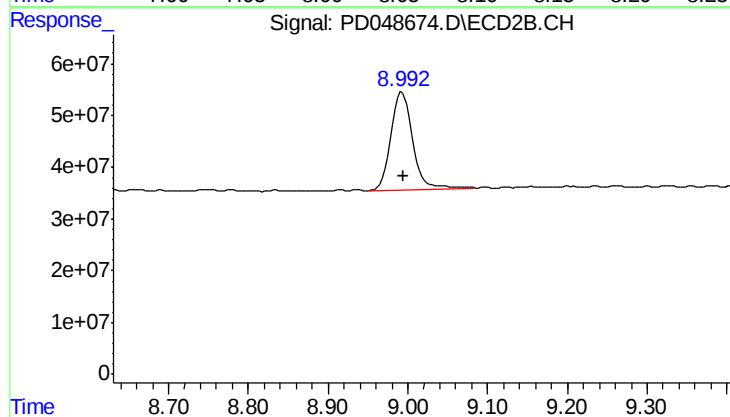

#7 Decachlorobiphenyl

R.T.: 8.993 min
Delta R.T.: 0.000 min
Response: 356441826
Conc: 21.72 ng/ml