

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080122\
 Data File : PD071275.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2022 19:01
 Operator : AR\AJ
 Sample : N3960-04
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RVE-152

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 08/02/2022
 Supervised By :mohammad ahmed 08/02/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 00:09:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 26 03:39:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	2.816	3.574	38444291	432.6E6	13.556	15.366
2) SA Decachlor...	8.018	9.106	36805249	145.1E6	13.270	14.012
Target Compounds						
12) B 4,4'-DDE	5.307	6.231	6007848	25371300	1.755	1.775m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080122\
Data File : PD071275.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2022 19:01
Operator : AR\AJ
Sample : N3960-04
Misc :
ALS Vial : 36 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
RVE-152


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 08/02/2022
Supervised By :mohammad ahmed 08/02/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 00:09:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072622.M
Quant Title : GC Extractables
QLast Update : Tue Jul 26 03:39:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

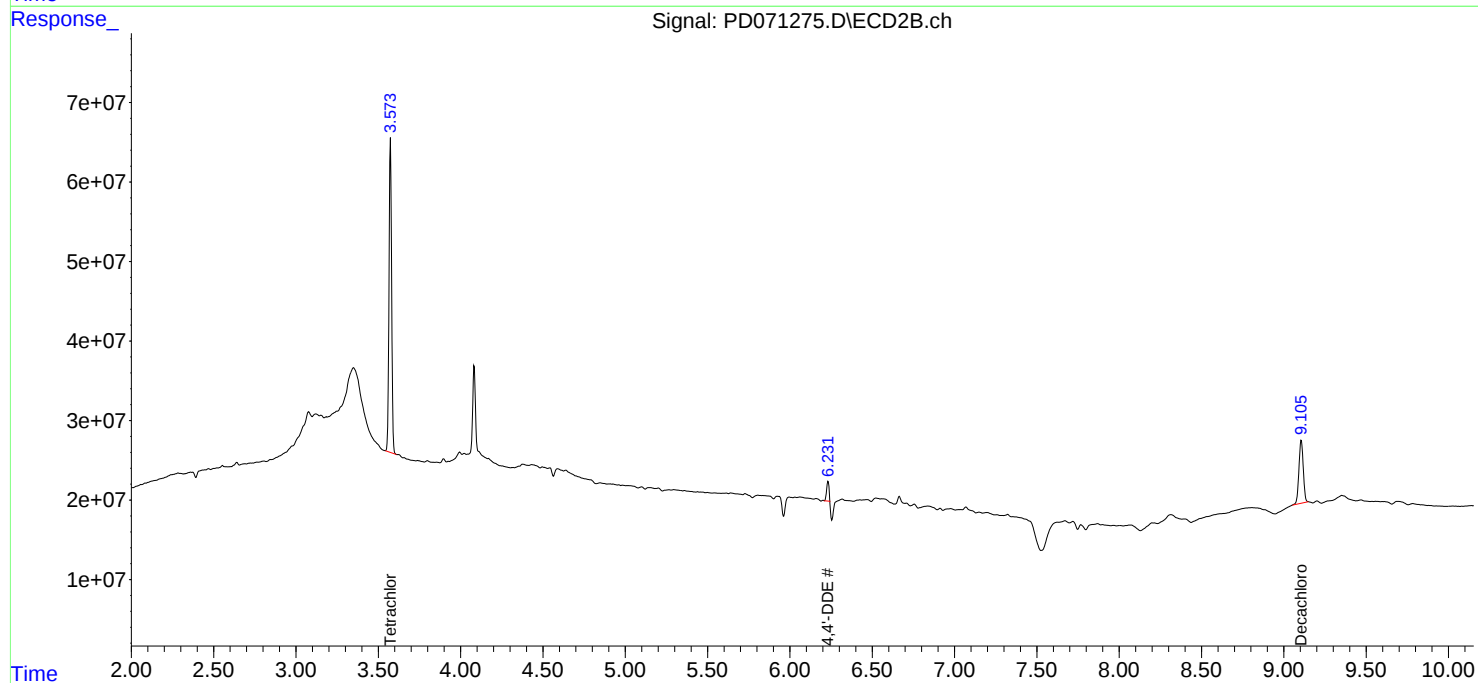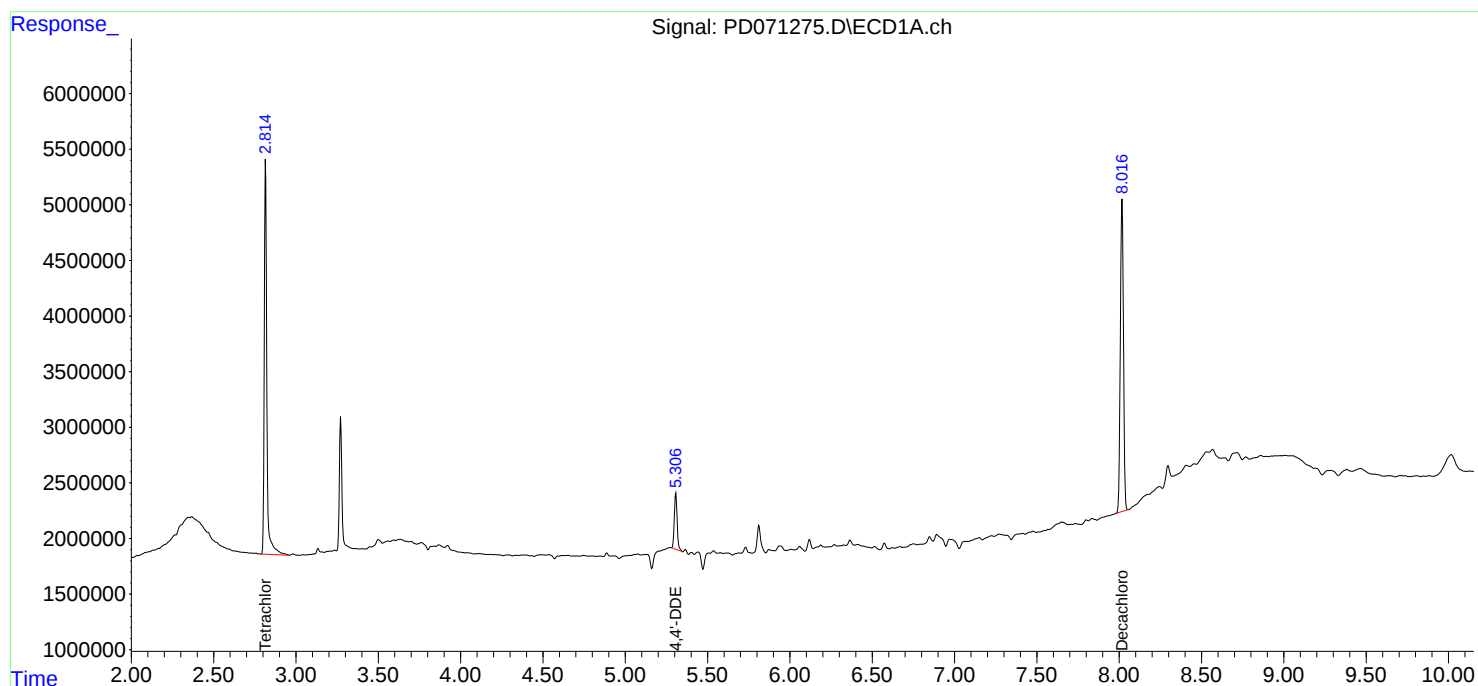

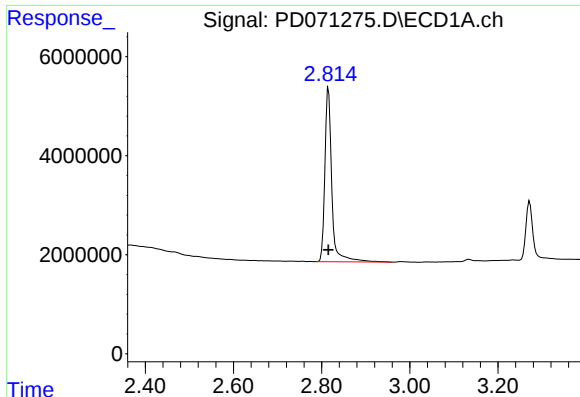


#1 Tetrachloro-m-xylene

R.T.: 2.816 min
Delta R.T.: 0.000 min
Response: 38444291
Conc: 13.56 ng/ml

Instrument :
ECD_D
ClientSampleId :
RVE-152


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 08/02/2022
Supervised By :mohammad ahmed 08/02/2022

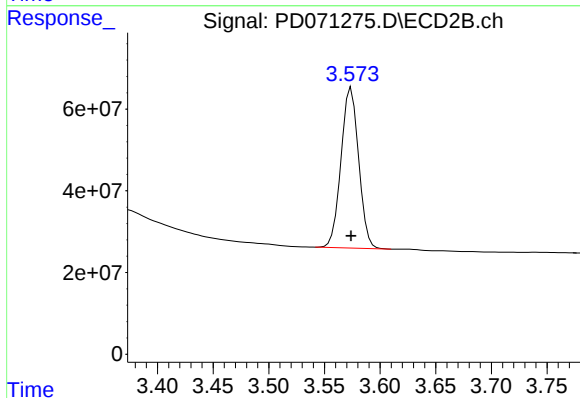


#1 Tetrachloro-m-xylene

R.T.: 3.574 min
Delta R.T.: 0.000 min
Response: 432555273
Conc: 15.37 ng/ml

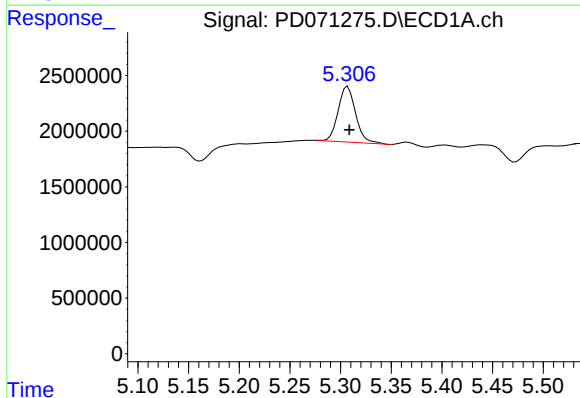


#12 4,4'-DDE

R.T.: 5.307 min
Delta R.T.: -0.002 min
Response: 6007848
Conc: 1.76 ng/ml

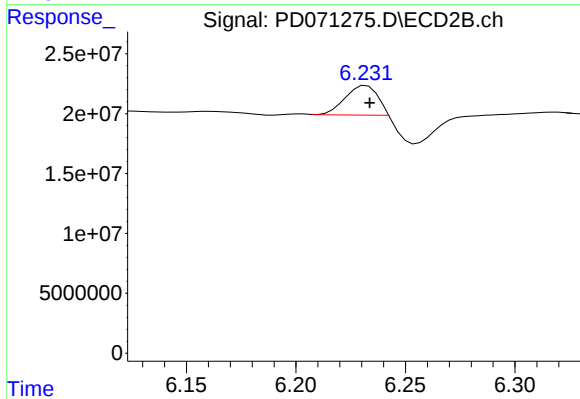

#12 4,4'-DDE

R.T.: 6.231 min
Delta R.T.: -0.003 min
Response: 25371300
Conc: 1.77 ng/ml m

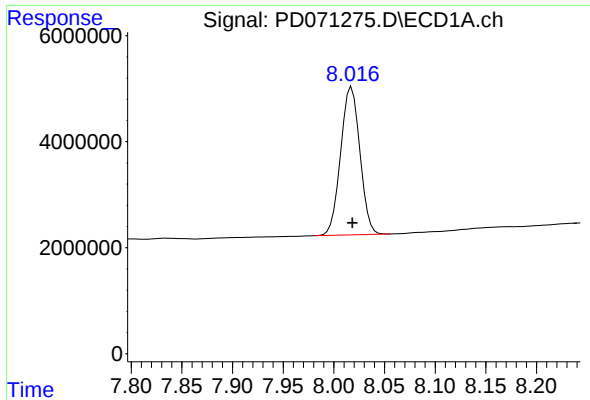


#28 Decachlorobiphenyl

R.T.: 8.018 min
Delta R.T.: 0.000 min
Response: 36805249
Conc: 13.27 ng/ml

Instrument :
ECD_D
ClientSampleId :
RVE-152

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 08/02/2022
Supervised By :mohammad ahmed 08/02/2022

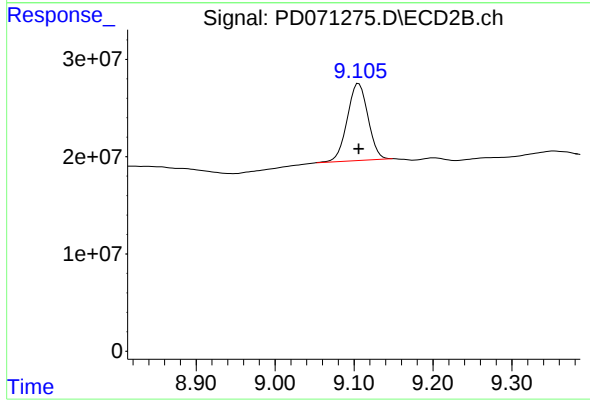

#28 Decachlorobiphenyl

R.T.: 9.106 min
Delta R.T.: 0.000 min
Response: 145056758
Conc: 14.01 ng/ml