

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080123\
 Data File : PD076958.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2023 11:32
 Operator : AR\AJ
 Sample : PIBLK222
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 21:30:28 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 14:58:34 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.551	2.763	48946759	25989576	23.008	24.348
27)	SA Decachlor...	9.092	7.906	127.0E6	59167457	52.295	55.195
Target Compounds							
5)	MB Aldrin	0.000	4.220	0	433414	N.D.	0.288
6)	B beta-BHC	0.000	3.849f	0	1601740	N.D.	2.236
7)	B delta-BHC	4.776	0.000	4975532	0	1.484	N.D. #
8)	B Heptachlo...	0.000	4.741	0	242978	N.D.	0.173
10)	B trans-Chl...	5.991	0.000	1769252	0	0.575	N.D. #
11)	B cis-Chlor...	5.991f	0.000	1769252	0	0.558	N.D. #
15)	B Endosulfa...	0.000	5.881f	0	329473	N.D.	0.274
18)	B Endrin al...	0.000	6.115	0	295015	N.D.	0.352


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080123\
Data File : PD076958.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2023 11:32
Operator : AR\AJ
Sample : PIBLK222
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 21:30:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

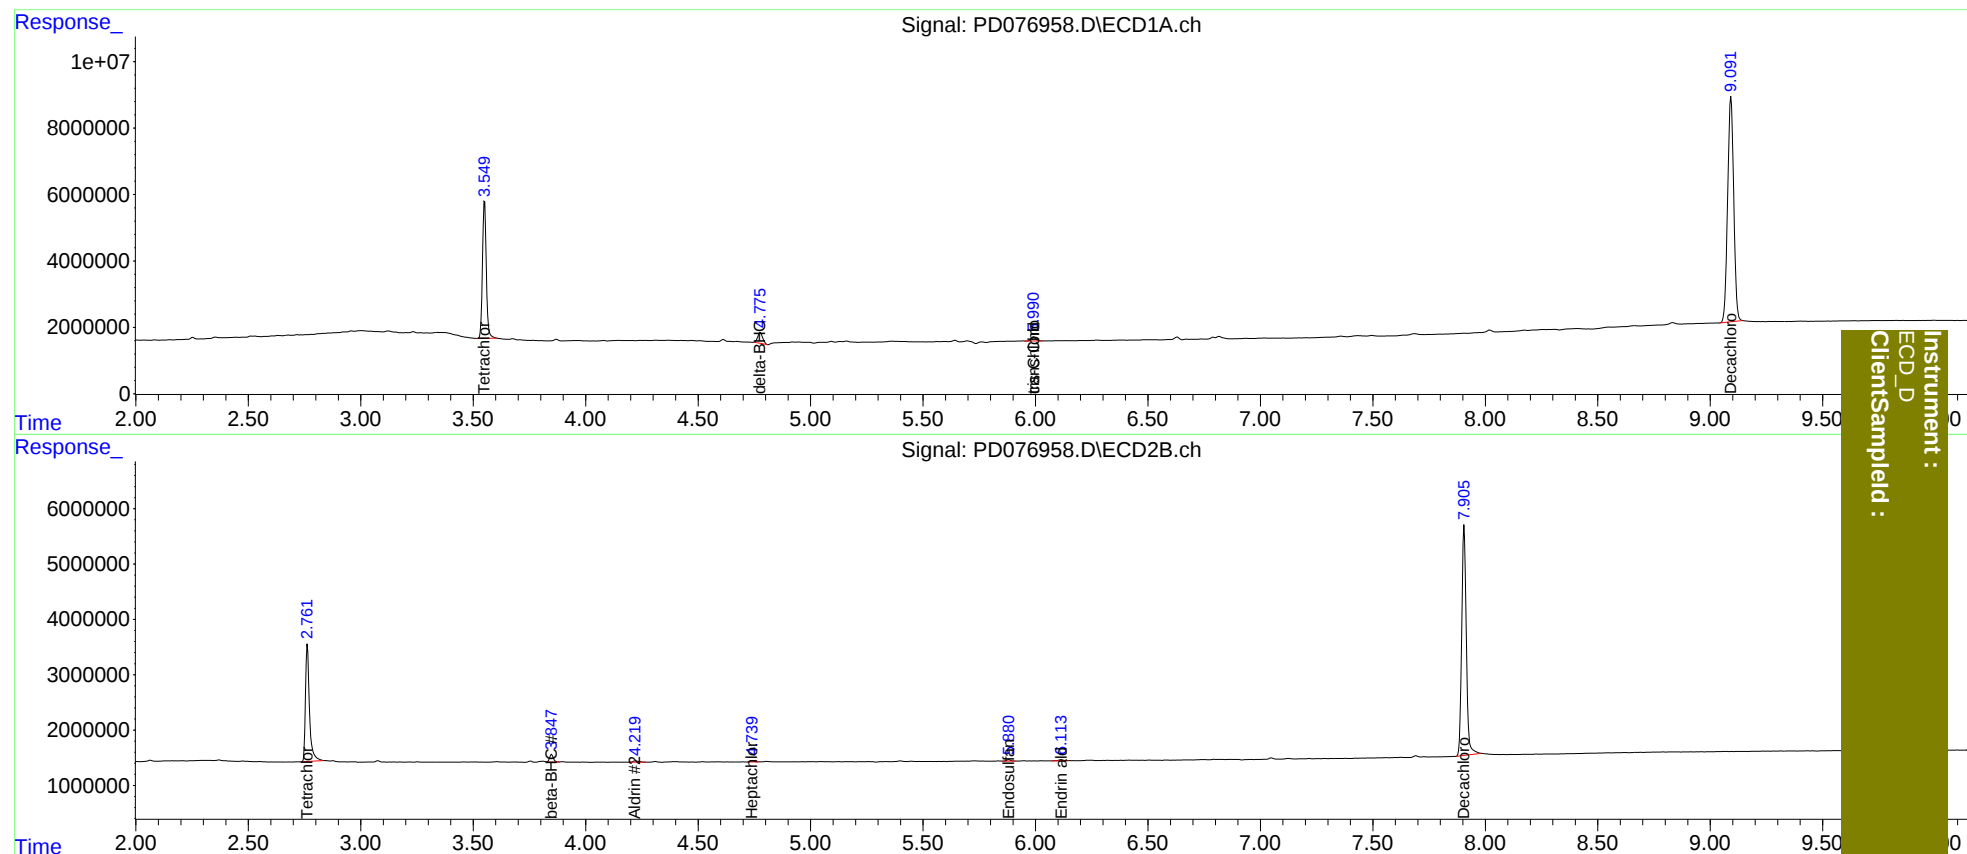


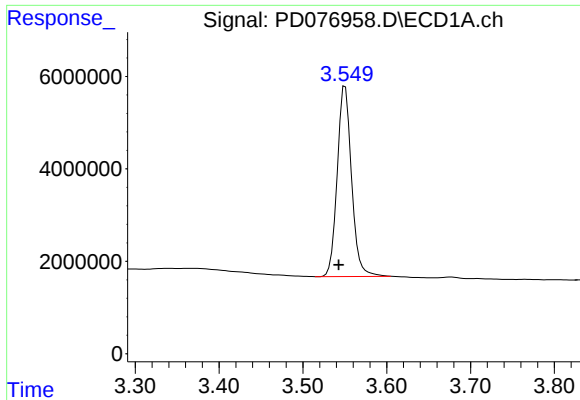

#1 Tetrachloro-m-xylene


R.T.: 3.551 min
Delta R.T.: 0.007 min
Response: 48946759
Conc: 23.01 ng/ml

Instrument :
ECD_D
ClientSampleId :

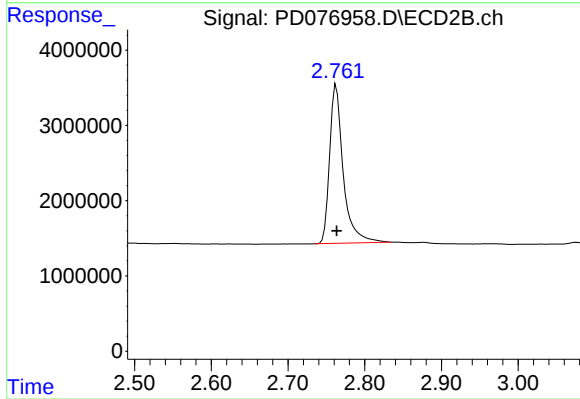


#1 Tetrachloro-m-xylene

R.T.: 2.763 min
Delta R.T.: 0.000 min
Response: 25989576
Conc: 24.35 ng/ml

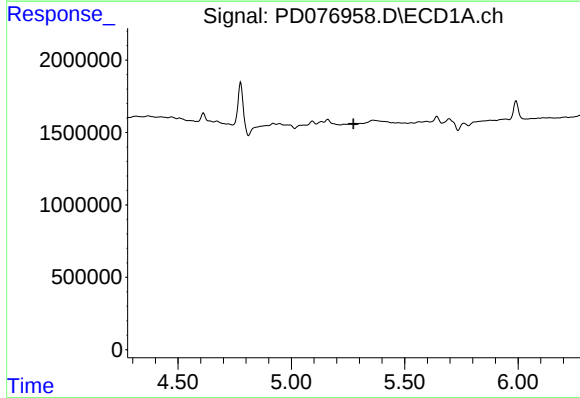


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.274 min
Response: 0
Conc: N.D.

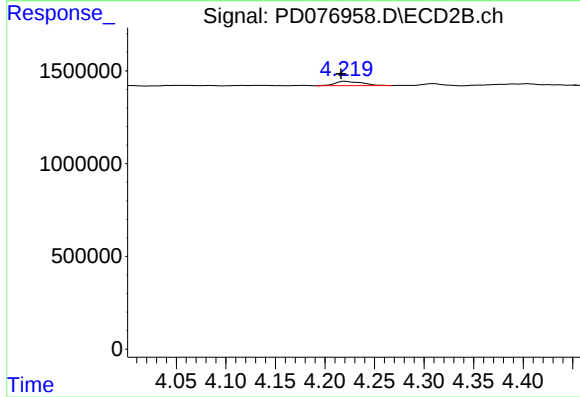

#5 Aldrin


R.T.: 4.220 min
Delta R.T.: 0.004 min
Response: 433414
Conc: 0.29 ng/ml

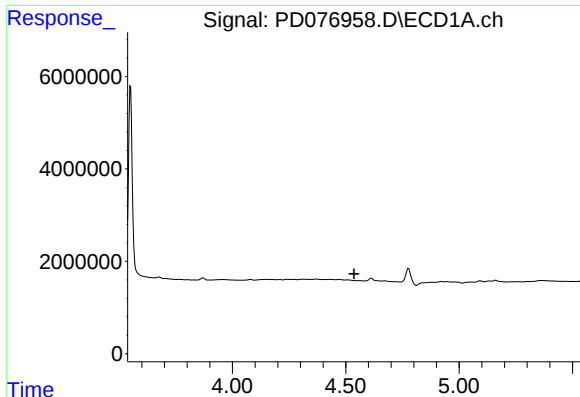

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.537 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

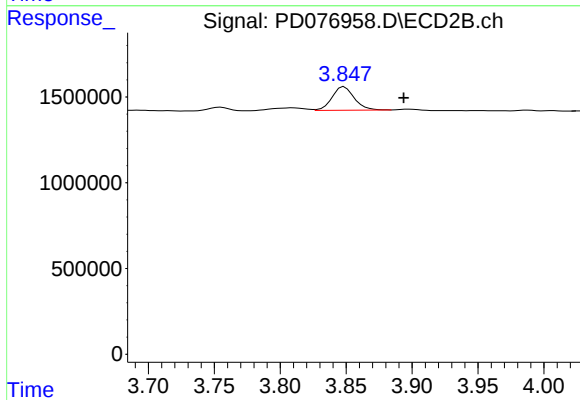


#6 beta-BHC

R.T.: 3.849 min
Delta R.T.: -0.045 min
Response: 1601740
Conc: 2.24 ng/ml

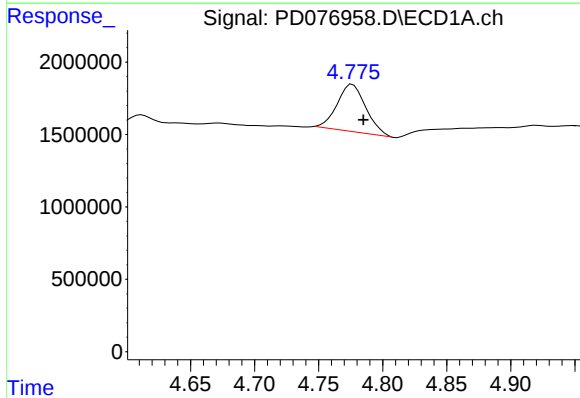


#7 delta-BHC

R.T.: 4.776 min
Delta R.T.: -0.009 min
Response: 4975532
Conc: 1.48 ng/ml

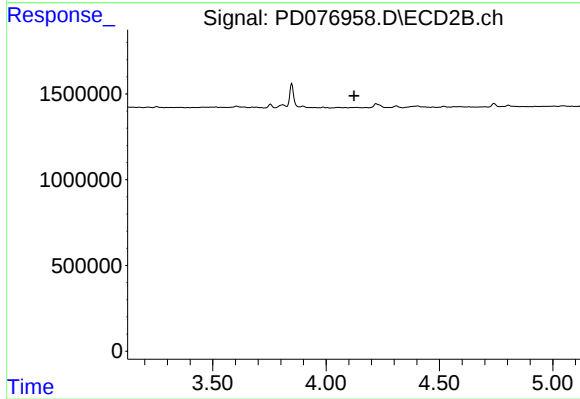

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.123 min
Response: 0
Conc: N.D.

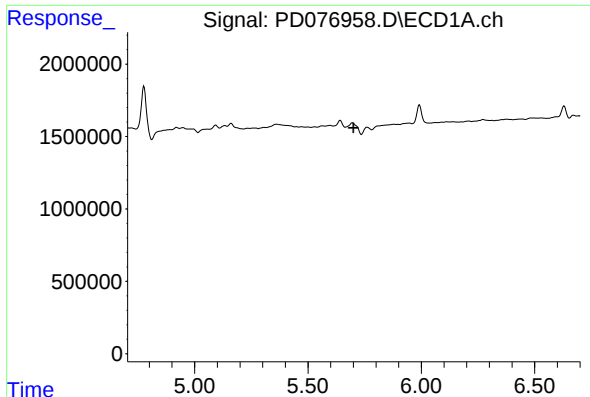

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.701 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

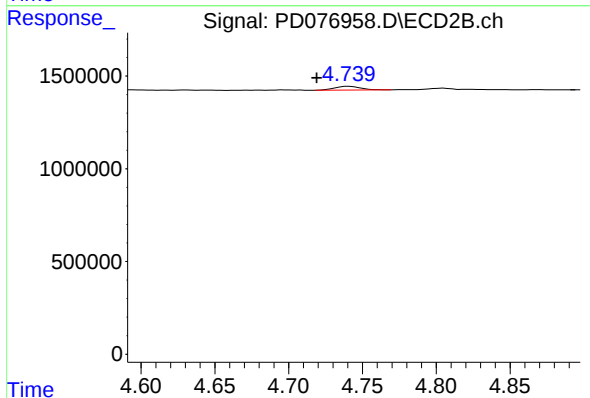


#8 Heptachlor epoxide

R.T.: 4.741 min
Delta R.T.: 0.022 min
Response: 242978
Conc: 0.17 ng/ml

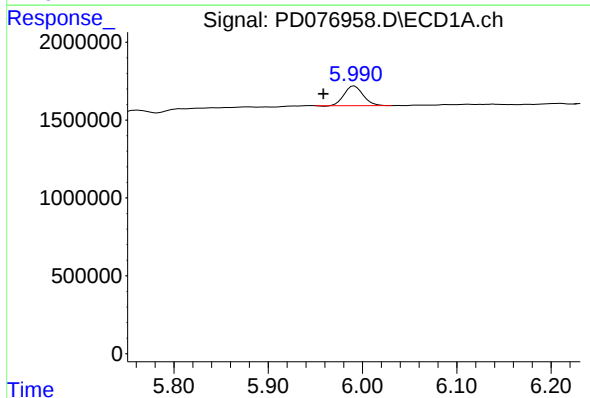


#10 trans-Chlordane

R.T.: 5.991 min
Delta R.T.: 0.033 min
Response: 1769252
Conc: 0.58 ng/ml

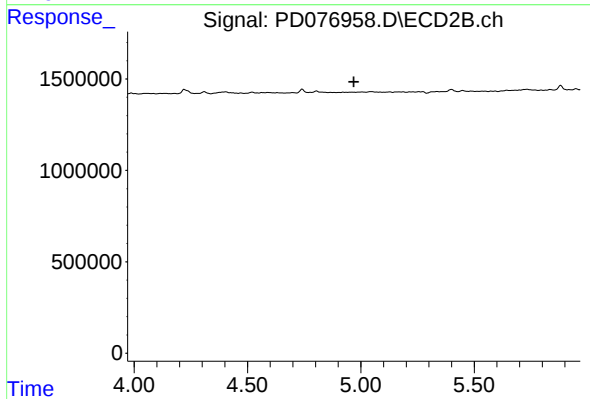

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 4.969 min
Response: 0
Conc: N.D.

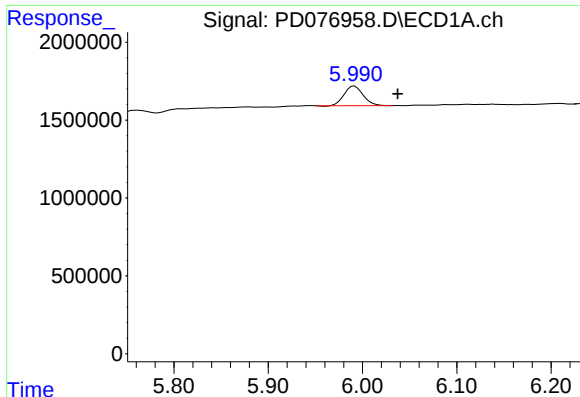

#11 cis-Chlordane


R.T.: 5.991 min
Delta R.T.: -0.046 min
Response: 1769252
Conc: 0.56 ng/ml

Instrument :
ECD_D
ClientSampleId :

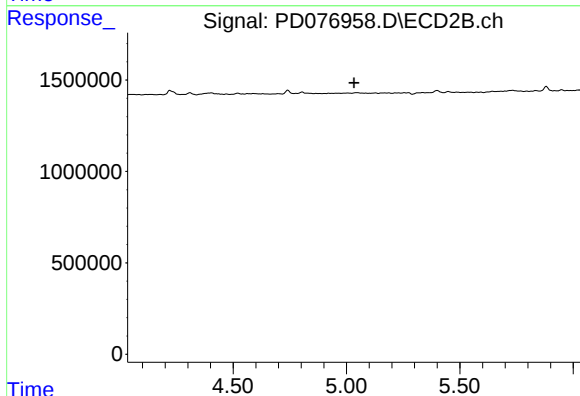


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.033 min
Response: 0
Conc: N.D.

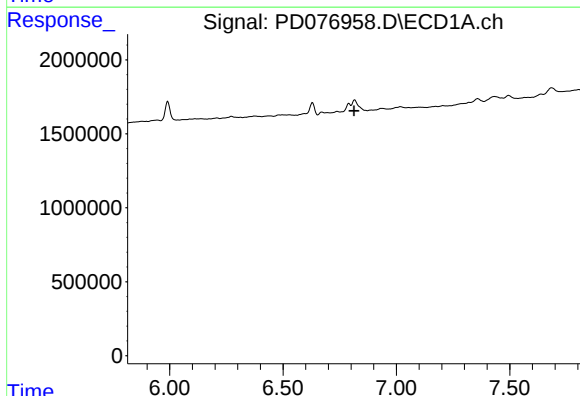


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.814 min
Response: 0
Conc: N.D.

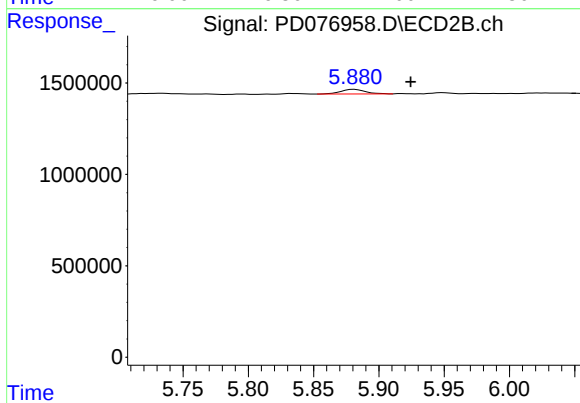

#15 Endosulfan II


R.T.: 5.881 min
Delta R.T.: -0.043 min
Response: 329473
Conc: 0.27 ng/ml

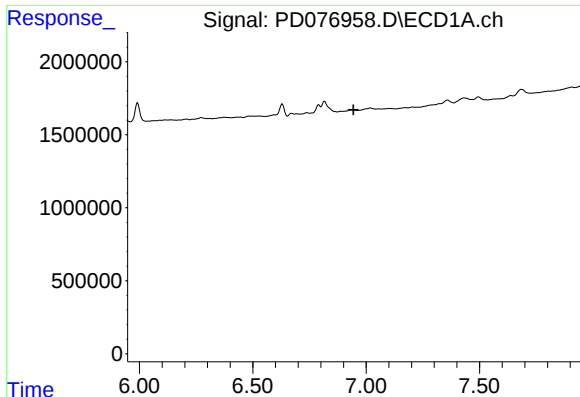

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.945 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

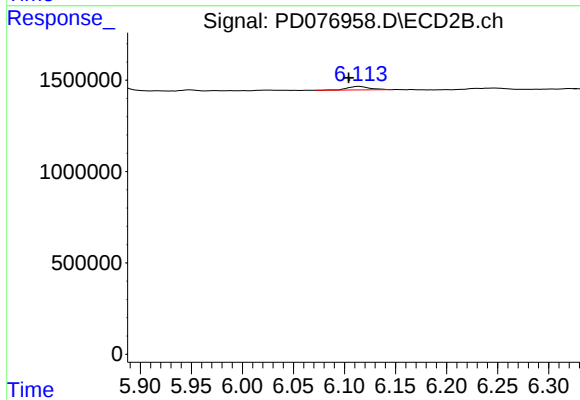


#18 Endrin aldehyde

R.T.: 6.115 min
Delta R.T.: 0.010 min
Response: 295015
Conc: 0.35 ng/ml

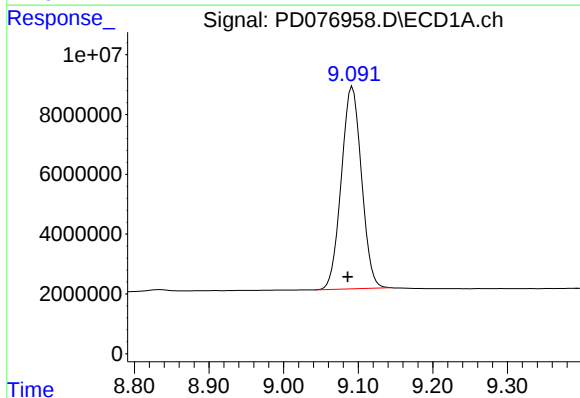

#27 Decachlorobiphenyl

R.T.: 9.092 min
Delta R.T.: 0.006 min
Response: 127049482
Conc: 52.29 ng/ml

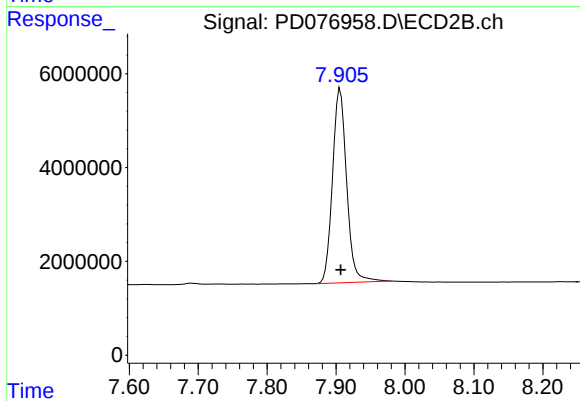

#27 Decachlorobiphenyl

R.T.: 7.906 min
Delta R.T.: 0.000 min
Response: 59167457
Conc: 55.19 ng/ml