

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080124\
 Data File : PD084172.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2024 12:23
 Operator : AR\AJ
 Sample : P3397-05MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BHCM6MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 01:12:44 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072424CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 25 11:17:53 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.561	2.771	17548332	104.3E6	19.599	19.994
27)	SA Decachlor...	9.113	7.894	39062880	121.2E6	20.352	21.021
Target Compounds							
2)	A alpha-BHC	4.019	3.270	92188451	450.2E6	55.407	52.665
3)	MA gamma-BHC...	4.353	3.598	92368941	417.3E6	55.916	53.198
4)	MA Heptachlor	4.944	3.936	98068017	422.6E6	53.385	54.498
5)	MB Aldrin	5.288	4.214	98685045	388.4E6	53.445	49.337
6)	B beta-BHC	4.551	3.895	37495025	176.8E6	50.167	49.486
7)	B delta-BHC	4.799	4.124	97526369	444.5E6	48.640	52.184
8)	B Heptachlo...	5.716	4.715	88066811	374.7E6	47.643	51.664
9)	A Endosulfan I	6.103	5.085	91481984	353.3E6	52.942	54.657
10)	B trans-Chl...	5.972	4.964	94857741	382.5E6	53.457	54.007
11)	B cis-Chlor...	6.052	5.028	95760161	384.4E6	52.482	53.179
12)	B 4,4'-DDE	6.224	5.216	194.6E6	729.7E6	105.801	106.214
13)	MA Dieldrin	6.379	5.348	205.2E6	763.2E6	110.204	107.700
14)	MA Endrin	6.609	5.624	174.0E6	655.2E6	109.147	107.430
15)	B Endosulfa...	6.829	5.917	179.4E6	625.4E6	102.105	104.175
16)	A 4,4'-DDD	6.743	5.770	148.8E6	568.6E6	113.462	108.663
17)	MA 4,4'-DDT	7.058	6.020	161.8E6	588.6E6	114.245	112.710
18)	B Endrin al...	6.960	6.097	135.4E6	483.2E6	107.982	109.198
19)	B Endosulfa...	7.195	6.319	174.0E6	610.0E6	106.982	106.269
20)	A Methoxychlor	7.534	6.595	425.2E6	1212.3E6	505.892	469.899
21)	B Endrin ke...	7.682	6.825	195.0E6	662.5E6	108.239	106.407

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080124\
Data File : PD084172.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2024 12:23
Operator : AR\AJ
Sample : P3397-05MS
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 01:12:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072424CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 25 11:17:53 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

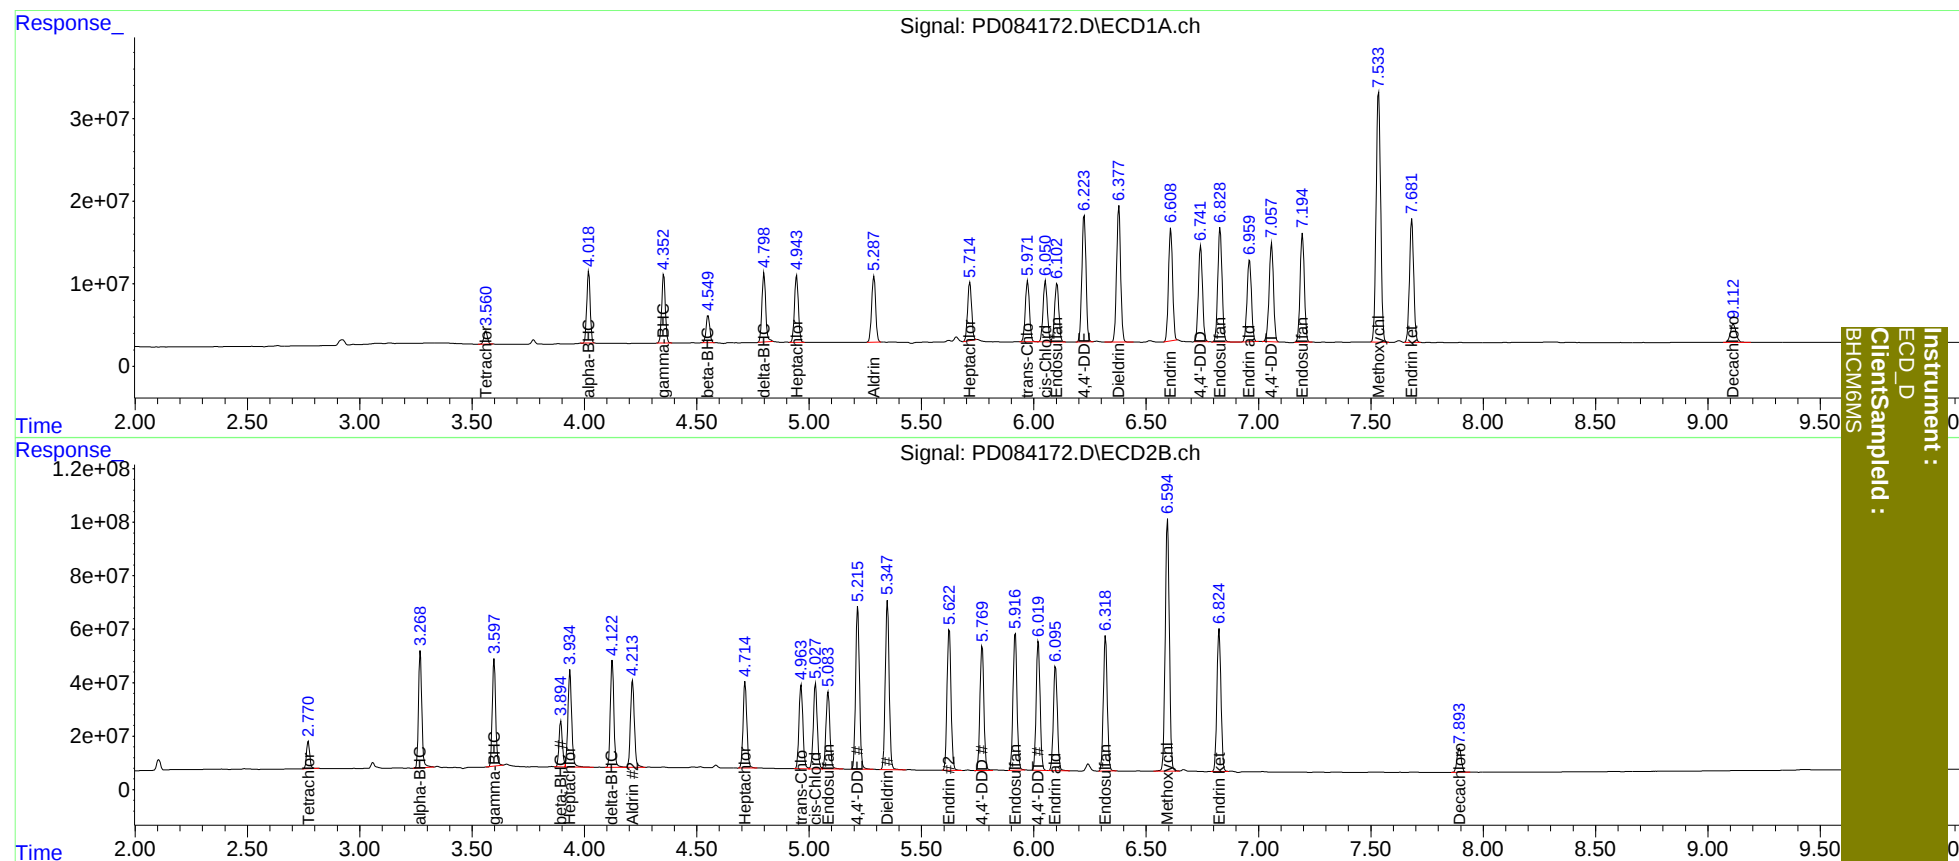

Instrument :
ECD_D
Client Sampled :
BHC6MS