

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080124\
 Data File : PD084173.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2024 12:36
 Operator : AR\AJ
 Sample : P3397-06MSD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BHCM6MSD

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/02/2024
 Supervised By :Ankita Jodhani 08/02/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 01:13:12 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072424CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 25 11:17:53 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.561	2.771	17645401	104.6E6	19.707	20.045
27)	SA Decachlor...	9.114	7.893	39321451	121.2E6	20.486	21.032
Target Compounds							
2)	A alpha-BHC	4.017	3.270	93035705	449.4E6	55.917m	52.573
3)	MA gamma-BHC...	4.352	3.597	92625425	434.9E6	56.071	55.437m
4)	MA Heptachlor	4.944	3.936	97981395	422.2E6	53.338	54.436
5)	MB Aldrin	5.287	4.214	98752406	387.4E6	53.482	49.219
6)	B beta-BHC	4.550	3.895	37543673	176.6E6	50.232	49.432
7)	B delta-BHC	4.797	4.124	100.3E6	442.7E6	50.021m	51.973
8)	B Heptachlo...	5.715	4.715	87956250	373.9E6	47.583	51.557
9)	A Endosulfan I	6.103	5.084	91476230	352.0E6	52.938	54.455
10)	B trans-Chl...	5.972	4.965	94957835	381.2E6	53.513	53.824
11)	B cis-Chlor...	6.052	5.028	95714324	383.3E6	52.457	53.017
12)	B 4,4'-DDE	6.224	5.216	194.8E6	729.0E6	105.932	106.108
13)	MA Dieldrin	6.378	5.348	205.1E6	761.0E6	110.139	107.386
14)	MA Endrin	6.610	5.623	174.1E6	655.4E6	109.260	107.470
15)	B Endosulfa...	6.829	5.917	179.2E6	623.1E6	102.010	103.777
16)	A 4,4'-DDD	6.743	5.770	148.8E6	567.4E6	113.419	108.440
17)	MA 4,4'-DDT	7.058	6.020	161.9E6	587.5E6	114.330	112.500
18)	B Endrin al...	6.959	6.097	135.4E6	480.9E6	107.968	108.672
19)	B Endosulfa...	7.195	6.319	173.4E6	609.2E6	106.590	106.127
20)	A Methoxychlor	7.535	6.595	424.8E6	1208.7E6	505.434	468.531
21)	B Endrin ke...	7.682	6.824	194.9E6	659.4E6	108.160	105.899

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080124\
Data File : PD084173.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2024 12:36
Operator : AR\AJ
Sample : P3397-06MSD
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 01:13:12 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072424CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 25 11:17:53 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

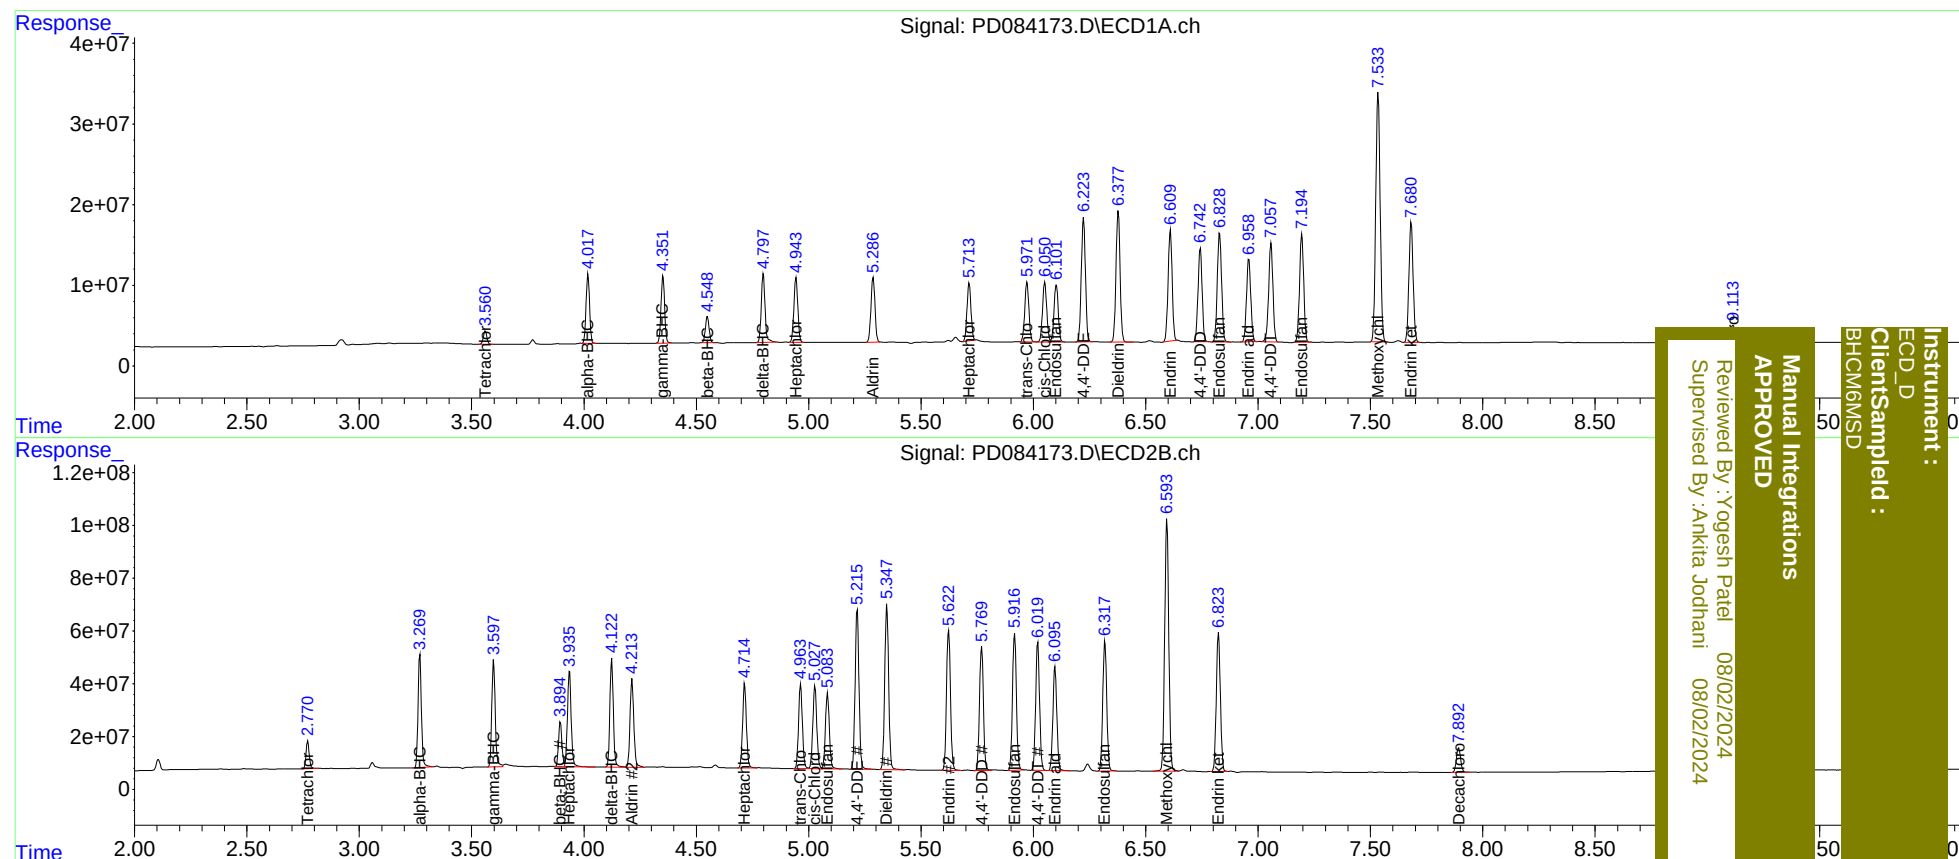

311.0
Reviewed By : Yogesh Patel 08/02/2024
Supervised By : Ankita Jodhani 08/02/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
BHC6MSD