

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080221\
 Data File : PD064674.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Aug 2021 17:45
 Operator : AR\AJ
 Sample : M3124-16
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0097

Manual Integrations
 APPROVED

mohammad
 8/3/2021 3:12:35 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 03 08:06:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 28 07:07:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	5.406	4.617	19731737	154.1E6	16.541	16.863m
27)	SA Decachlor...	11.307	10.360	36466442	173.0E6	27.702	29.089
Target Compounds							
12)	B 4,4'-DDE	8.437	7.608	2166138	30932799	1.503	4.100 #
13)	MA Dieldrin	8.571	7.737	8586121	51780840	5.758	6.447m
14)	MA Endrin	8.816	8.034	4868540	101.9E6	3.802m	17.737m#
15)	B Endosulfa...	9.031	8.335	8827094	44550502	6.797	7.718
16)	A 4,4'-DDD	8.960	8.176	45763776	54729621	37.281m	9.502m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080221\
Data File : PD064674.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Aug 2021 17:45
Operator : AR\AJ
Sample : M3124-16
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 03 08:06:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 28 07:07:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

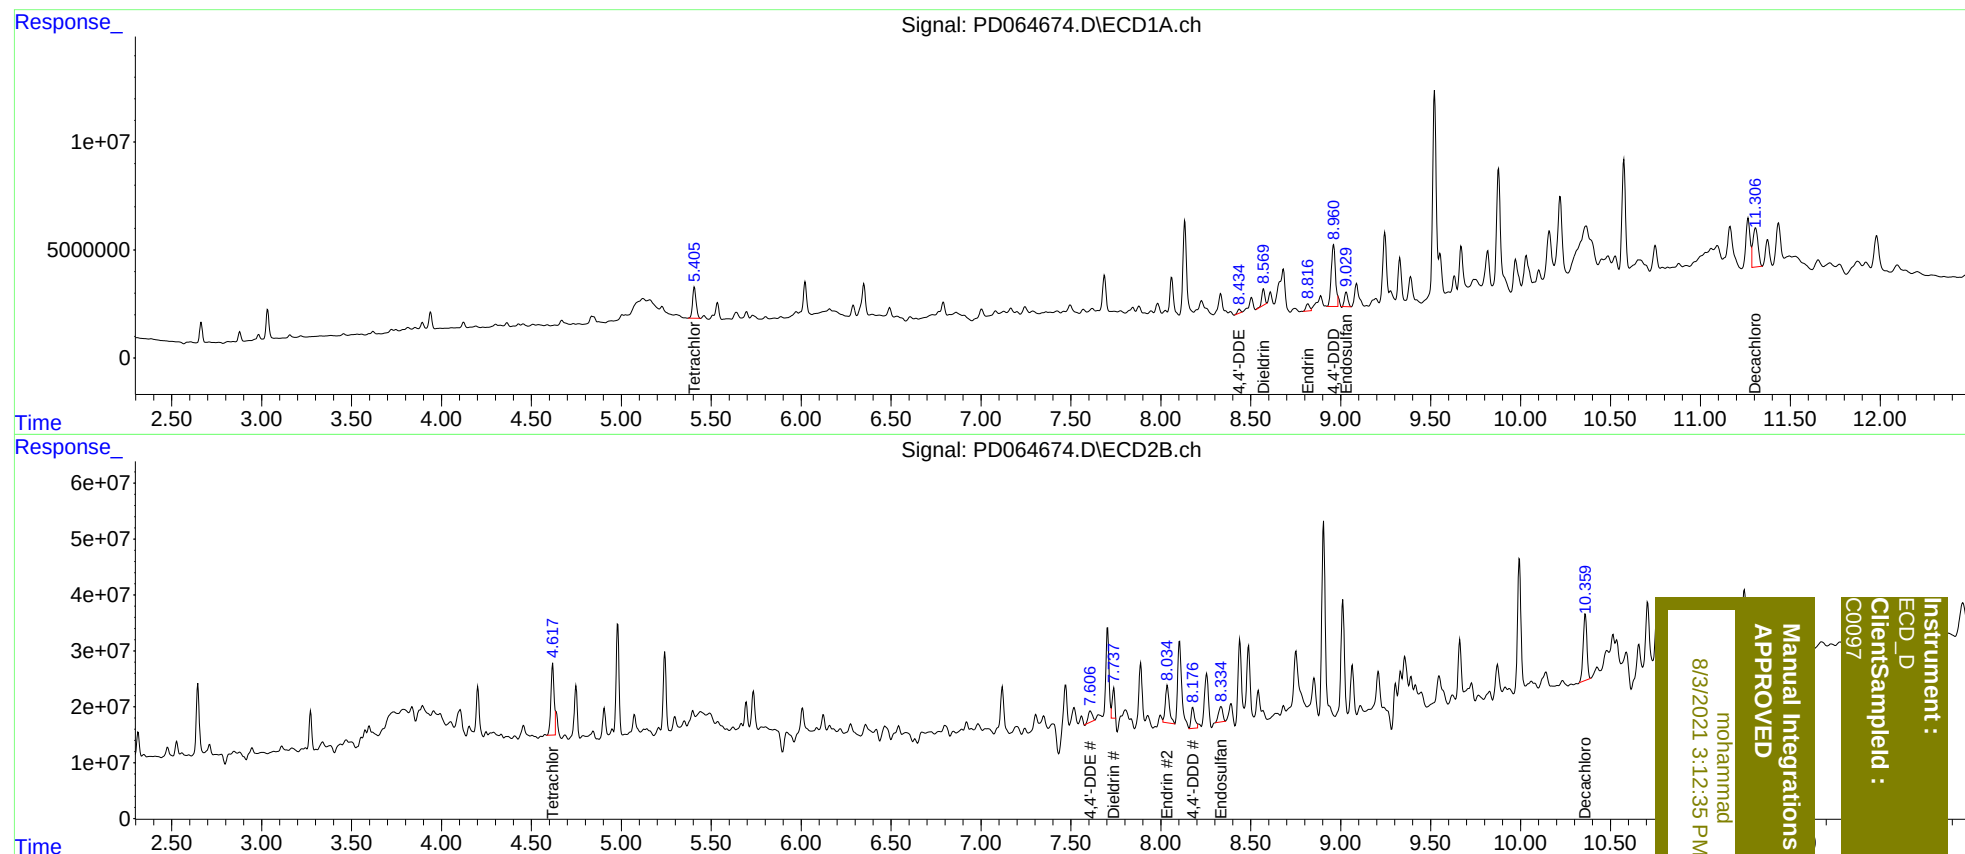

Manual Integrations
APPROVED

mohammad
8/3/2021 3:12:35 PM

Instrument :
ECD_D
ClientSampled :
C0097