

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080221\
 Data File : PD064660.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Aug 2021 14:02
 Operator : AR\AJ
 Sample : M3124-07MS
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleID :
 C0089MS

Manual Integrations
 APPROVED

mohammad
 8/3/2021 3:12:01 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 03 02:50:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 28 07:07:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	5.405	4.618	11278335	113.6E6	9.455	12.434 #
27)	SA Decachlor...	11.304	10.361	12518325	68677720	9.510m	11.549
Target Compounds							
2)	A alpha-BHC	5.987	5.319	106.5E6	842.5E6	65.377	68.355m
3)	MA gamma-BHC...	6.384	5.740	98506535	708.4E6	62.809	62.120
4)	MA Heptachlor	7.034	6.148	95409215	690.2E6	56.771	60.872m
5)	MB Aldrin	7.404	6.473	90105351	639.3E6	57.204	60.771
6)	B beta-BHC	6.643	6.115	41523481	312.0E6	53.224	51.433m
7)	B delta-BHC	6.908	6.377	99398220	653.3E6	57.120	60.134
8)	B Heptachlo...	7.873	7.047	85715355	507.8E6	49.926	54.859
9)	A Endosulfan I	8.276	7.449	75312754	424.8E6	53.426m	55.244
10)	B trans-Chl...	8.143	7.322	100.7E6	524.2E6	62.813	57.791
11)	B cis-Chlor...	8.223	7.392	84755379	504.3E6	54.396m	56.687
12)	B 4,4'-DDE	8.420	7.603	152.3E6	834.0E6	105.684	110.536
13)	MA Dieldrin	8.568	7.732	172.5E6	845.8E6	115.662	105.302m
14)	MA Endrin	8.807	8.023	146.7E6	700.6E6	114.553	121.958
15)	B Endosulfa...	9.043	8.333	141.0E6	609.3E6	108.557	105.558
16)	A 4,4'-DDD	8.961	8.186	146.6E6	632.2E6	119.397	109.770
17)	MA 4,4'-DDT	9.278	8.445	146.3E6	609.2E6	112.092	110.677m
18)	B Endrin al...	9.178	8.520	121.2E6	458.1E6	106.988	92.824
19)	B Endosulfa...	9.417	8.750	142.2E6	573.1E6	103.176	106.325
20)	A Methoxychlor	9.770	9.039	383.7E6	1327.8E6	536.179	518.564
21)	B Endrin ke...	9.913	9.269	166.4E6	615.6E6	110.007	102.622

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080221\
Data File : PD064660.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Aug 2021 14:02
Operator : AR\AJ
Sample : M3124-07MS
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 03 02:50:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 28 07:07:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

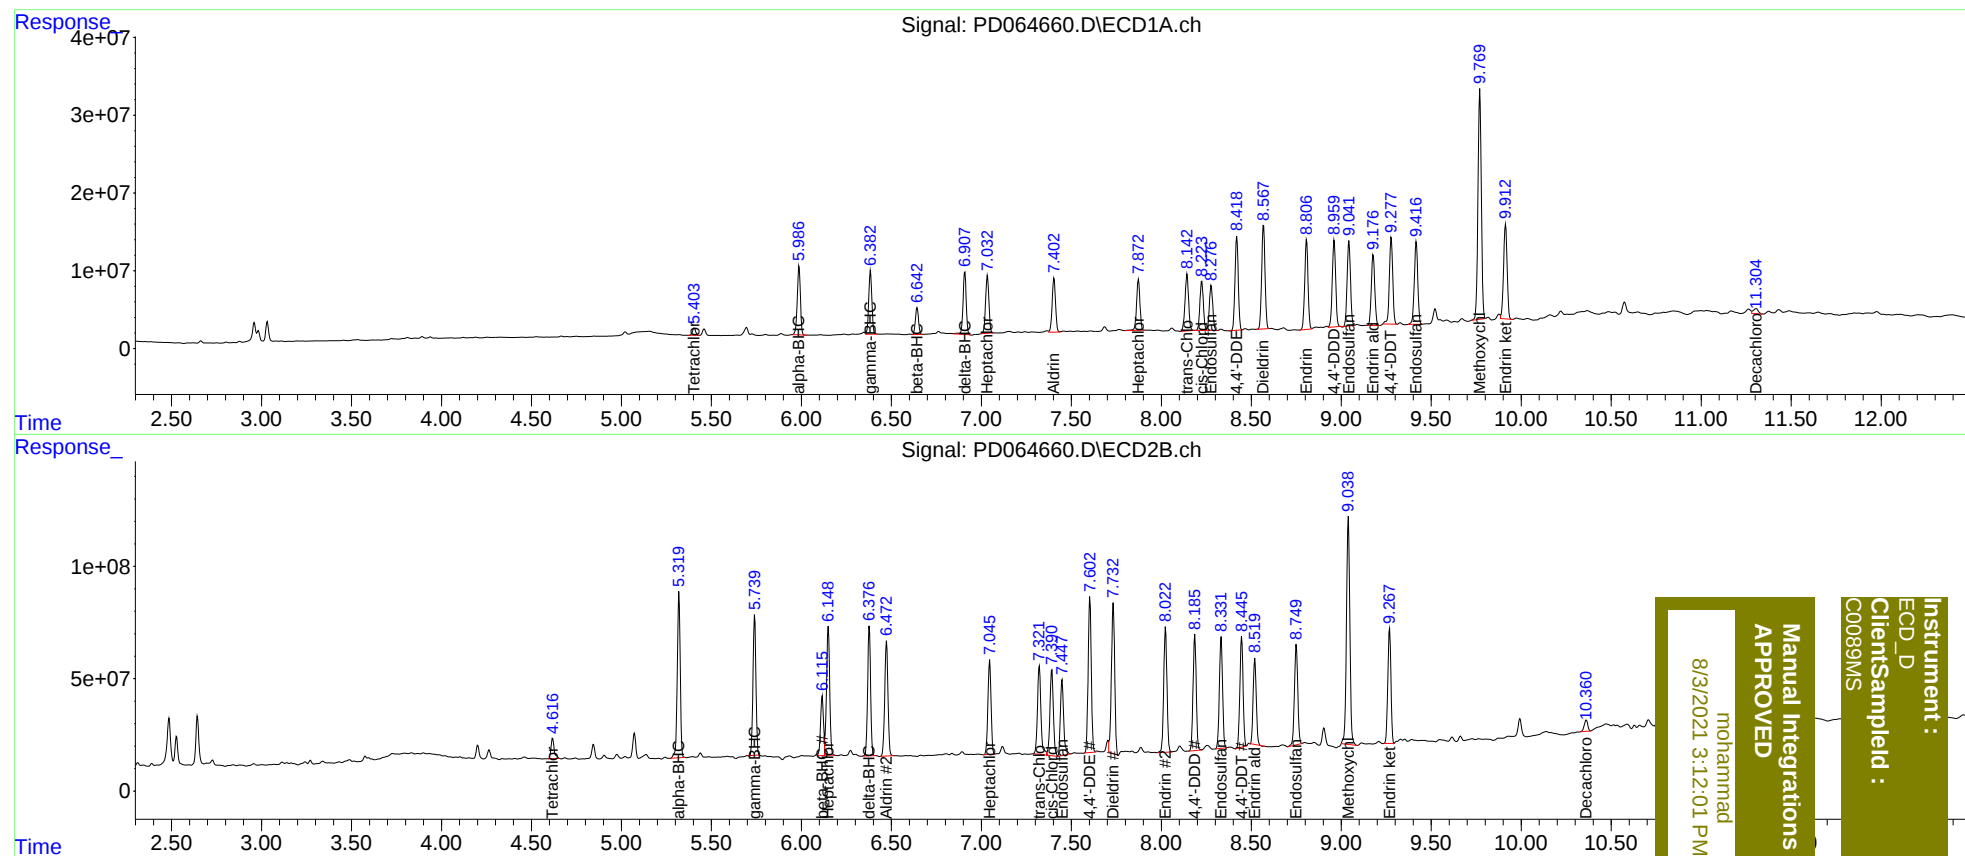

8/3/2021 3:12:01 PM
mohammad

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
C0089MS