

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080221\
 Data File : PD064662.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Aug 2021 14:34
 Operator : AR\AJ
 Sample : M3124-09
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0090

Manual Integrations
 APPROVED

mohammad
 8/3/2021 4:25:20 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 03 07:32:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 28 07:07:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	5.405	4.618	15350636	136.0E6	12.868	14.885
27)	SA Decachlor...	11.305	10.361	21235693	120.8E6	16.132	20.321 #
Target Compounds							
8)	B Heptachlo...	7.875	7.046	3237339	9497687	1.886	1.026 #
13)	MA Dieldrin	8.570	7.736	3840277	33068607	2.575	4.117m#
14)	MA Endrin	8.816	8.034	2159980	14337092	1.687	2.496m#
15)	B Endosulfa...	9.030	8.333	3469182	21687720	2.671	3.757 #
16)	A 4,4'-DDD	8.958	8.176	22688168	35785579	18.483m	6.213 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080221\
Data File : PD064662.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Aug 2021 14:34
Operator : AR\AJ
Sample : M3124-09
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 03 07:32:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 28 07:07:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

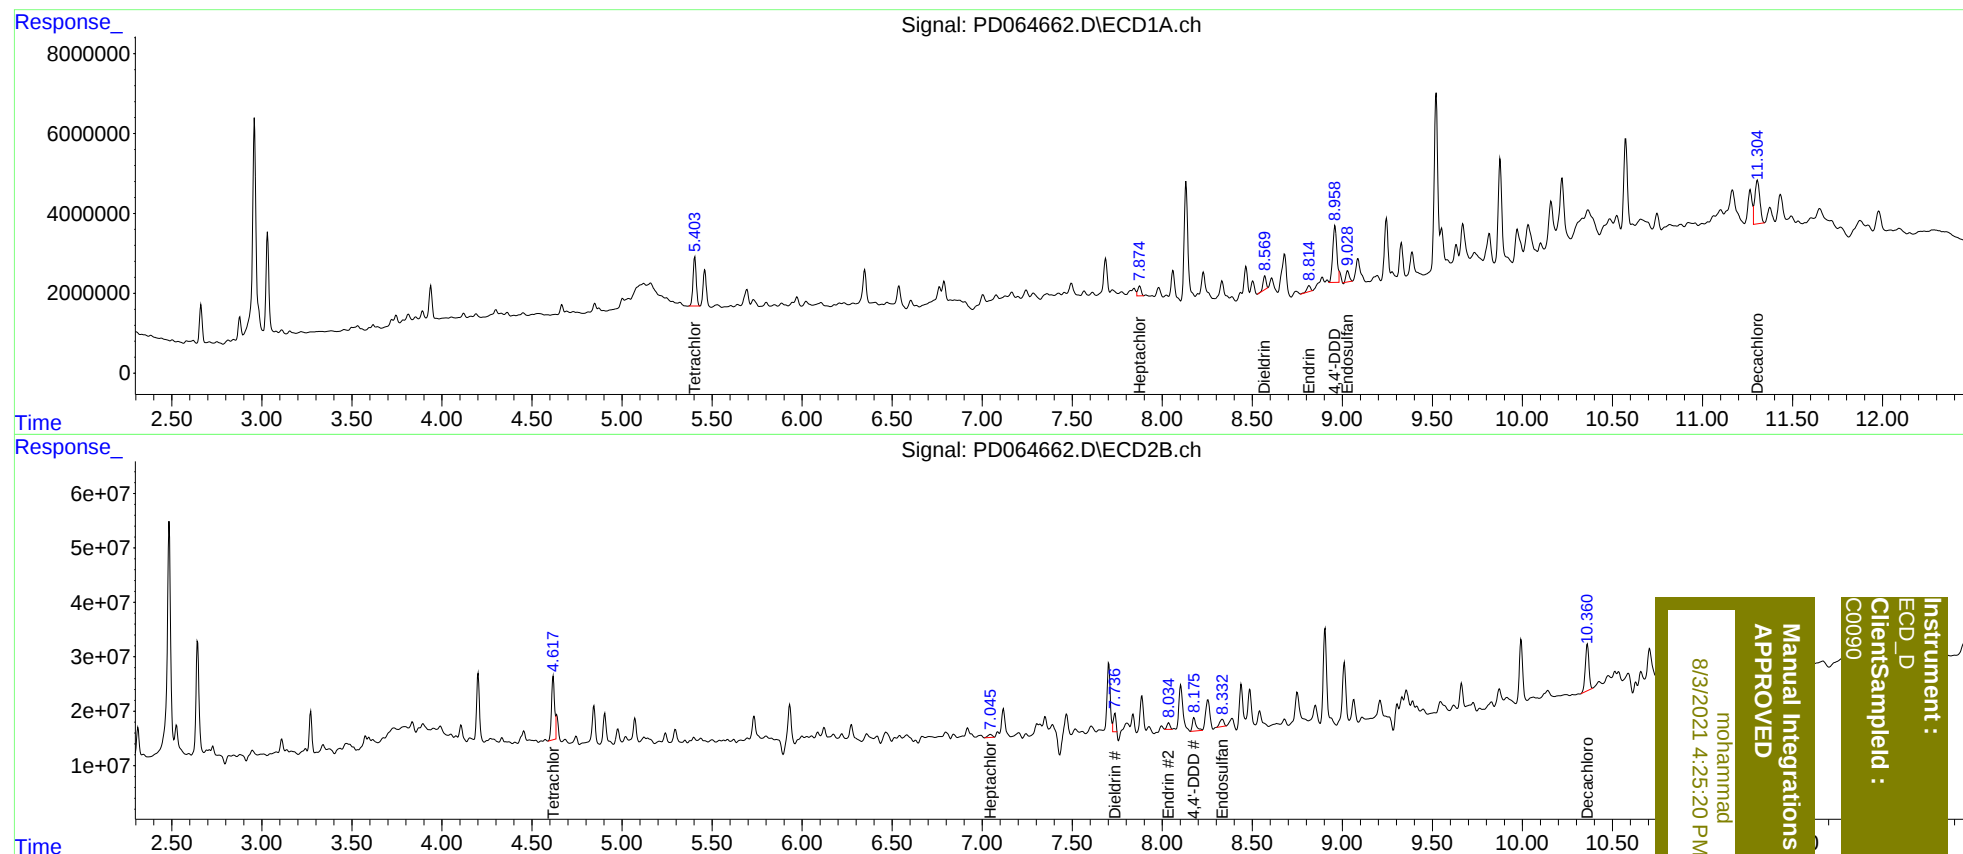

8/3/2021 4:25:20 PM

Manual Integrations
APPROVED

mohammad

Instrument :
ECD_D
ClientSampled :
C0090