

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080223\
 Data File : PD076966.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Aug 2023 09:43
 Operator : AR\AJ
 Sample : 03805-04
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 X3H48

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/03/2023
 Supervised By :Ankita Jodhani 08/04/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 22:07:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 14:58:34 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.551	2.763	59492981	23569172	27.966	22.081
27)	SA Decachlor...	9.094	7.906	91571117	43571090	37.692	40.646
Target Compounds							
2)	A alpha-BHC	4.010	3.265	6346.5E6	2626.7E6	1790.541	1659.969
3)	MA gamma-BHC...	4.343	3.595	6481.0E6	2643.5E6	1953.859	1764.517
4)	MA Heptachlor	4.934	3.934	913.2E6	413.4E6	262.677	276.514
5)	MB Aldrin	5.277	4.215	897.5E6	410.8E6	262.482	272.963
6)	B beta-BHC	4.540	3.892	2017.8E6	895.2E6	1327.532	1249.632
7)	B delta-BHC	4.787	4.122	4149.0E6	1667.4E6	1237.251m	1092.439
8)	B Heptachlo...	5.702	4.717	2312.7E6	1005.2E6	771.857m	714.481
9)	A Endosulfan I	6.091	5.087	5315.9E6	2174.4E6	1866.429	1754.959
10)	B trans-Chl...	5.960	4.967	3447.4E6	1439.1E6	1121.165	1064.244
11)	B cis-Chlor...	6.040	5.031	476.4E6	211.5E6	150.267	149.900
12)	B 4,4'-DDE	6.213	5.220	2878.3E6	1139.3E6	987.974	942.637
13)	MA Dieldrin	6.367	5.352	4958.7E6	2002.8E6	1571.565	1436.226
14)	MA Endrin	6.596	5.628	902.9E6	407.7E6	350.237	329.695
15)	B Endosulfa...	6.817	5.922	3136.2E6	1311.1E6	1179.530	1090.127
16)	A 4,4'-DDD	6.731	5.775	2280.3E6	831.3E6	1009.183	877.215
17)	MA 4,4'-DDT	7.045	6.026	1717.1E6	679.4E6	769.033	725.227
18)	B Endrin al...	6.946	6.102	2153.6E6	914.9E6	1151.728	1090.683
19)	B Endosulfa...	7.182	6.325	4443.6E6	1783.3E6	1779.344	1598.304
20)	A Methoxychlor	7.521	6.602	1435.2E6	485.4E6	1084.221	909.477
21)	B Endrin ke...	7.668	6.831	4292.0E6	1716.2E6	1550.152	1341.222

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080223\
Data File : PD076966.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Aug 2023 09:43
Operator : AR\AJ
Sample : 03805-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 22:07:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

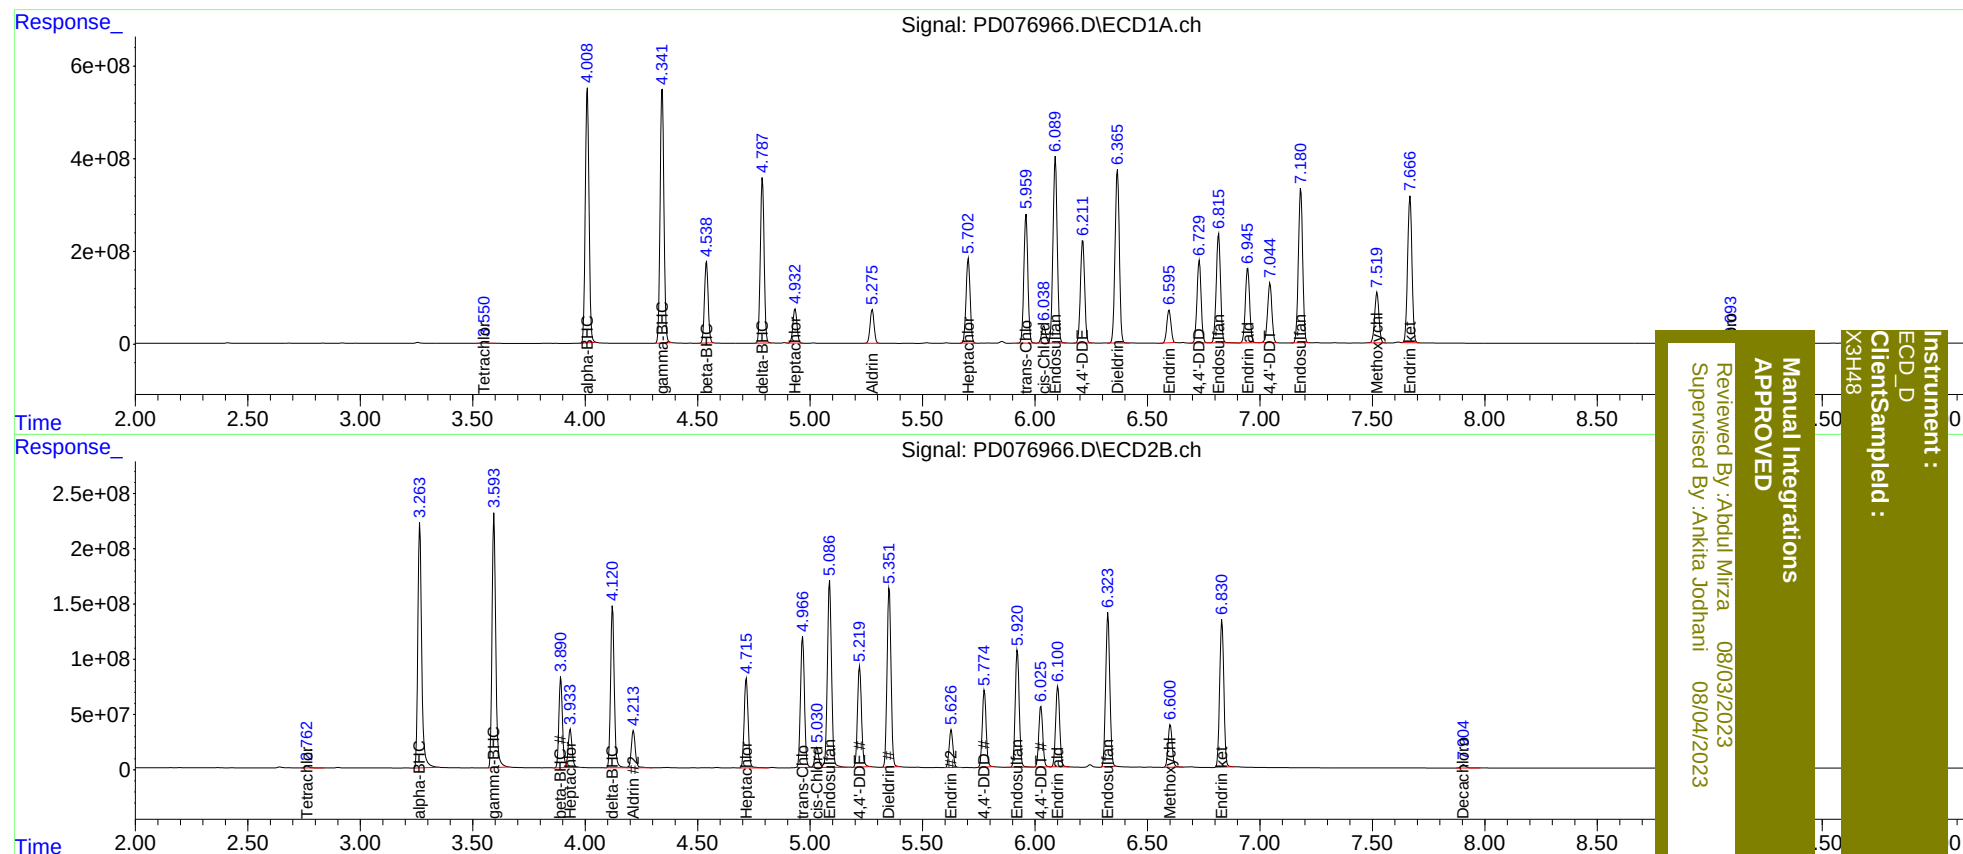

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 08/03/2023
Supervised By: Ankita Jodhani 08/04/2023

Instrument :
ECD_D
ClientSampled :
X3H48