

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080223\
 Data File : PD076965.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Aug 2023 09:12
 Operator : AR\AJ
 Sample : PB154563BS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS563

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/03/2023
 Supervised By :Ankita Jodhani 08/04/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 22:06:36 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 14:58:34 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.552	2.763	41454001	21617908	19.486	20.253
27)	SA Decachlor...	9.094	7.906	100.7E6	47869116	41.435	44.655
Target Compounds							
2)	A alpha-BHC	4.008	3.265	17151763	8113875	4.839	5.128
3)	MA gamma-BHC...	4.341	3.594	16105184	7597085	4.855	5.071
4)	MA Heptachlor	4.933	3.934	17674261	8110397	5.084	5.424
5)	MB Aldrin	5.276	4.214	17847783	8613929	5.220	5.724
6)	B beta-BHC	4.539	3.892	8165491	4108041	5.372	5.734
7)	B delta-BHC	4.785	4.121	20937957	6615953	6.244m	4.335 #
8)	B Heptachlo...	5.701	4.716	18664800	7605033	6.229m	5.406
9)	A Endosulfan I	6.090	5.087	15727718	6915427	5.522	5.582
10)	B trans-Chl...	5.960	4.967	16954263	7436011	5.514	5.499
11)	B cis-Chlor...	6.039	5.031	16652731	7658293	5.253	5.428
12)	B 4,4'-DDE	6.211	5.220	29085922	12454595	9.984	10.305
13)	MA Dieldrin	6.365	5.351	33589166	14384639	10.645	10.315
14)	MA Endrin	6.596	5.627	24971910	12594244	9.687	10.185
15)	B Endosulfa...	6.815	5.922	29345222	13058185	11.037	10.857
16)	A 4,4'-DDD	6.730	5.775	23854654	9496845	10.557	10.021
17)	MA 4,4'-DDT	7.044	6.026	21097344	8621333	9.449	9.203
18)	B Endrin al...	6.946	6.101	21990613	10386094	11.761	12.382
19)	B Endosulfa...	7.181	6.324	25667666	12056277	10.278	10.806
20)	A Methoxychlor	7.520	6.602	62756466	23207839	47.409	43.488
21)	B Endrin ke...	7.667	6.831	30176299	14138844	10.899	11.050

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080223\
Data File : PD076965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Aug 2023 09:12
Operator : AR\AJ
Sample : PB154563BS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 22:06:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

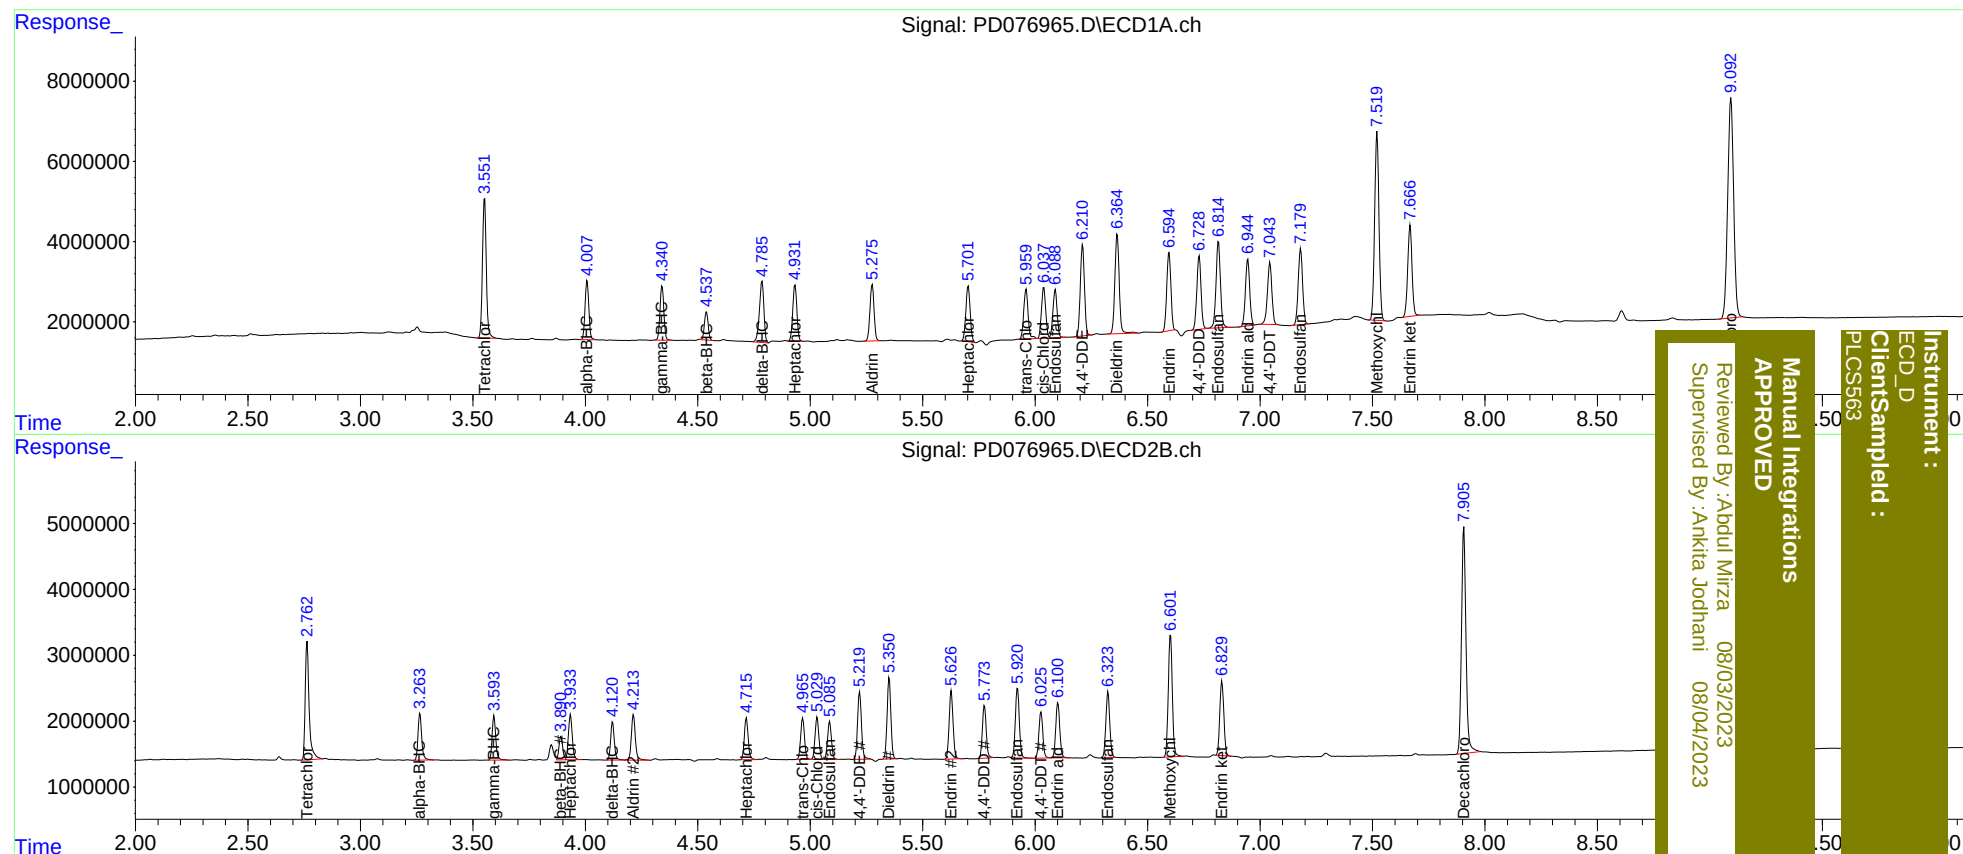

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 08/03/2023
Supervised By: Ankita Jodhani 08/04/2023

Instrument :
ECD_D
Client Sampled :
PLCS563