

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080223\
 Data File : PD076975.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Aug 2023 12:17
 Operator : AR\AJ
 Sample : 03805-09DL2 10X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 X3H68DL2

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 08/04/2023
 Supervised By : Ankita Jodhani 08/04/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 22:12:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 14:58:34 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	2.763	4301666	2440714	2.022	2.287
27)	SA Decachlor...	9.090	7.905	9132952	4635899	3.759	4.325
Target Compounds							
2)	A alpha-BHC	4.005	3.265	170.5E6	79943652	48.100	50.522
3)	MA gamma-BHC...	4.338	3.595	105.2E6	50427890	31.719	33.661
4)	MA Heptachlor	4.930	3.934	271.2E6	123.3E6	78.013	82.440
5)	MB Aldrin	5.272	4.214	155.8E6	71935720	45.577	47.799
6)	B beta-BHC	4.536	3.892	106.3E6	50604540	69.961	70.639
7)	B delta-BHC	4.783	4.122	186.0E6	86081031	55.467m	56.398
8)	B Heptachlo...	5.698	4.717	88001527	40976215	29.371m	29.126
9)	A Endosulfan I	6.087	5.087	140.3E6	65552067	49.263	52.908
10)	B trans-Chl...	5.956	4.967	144.0E6	66572449	46.828	49.231
11)	B cis-Chlor...	6.036	5.031	89391013	40601707	28.197	28.779
12)	B 4,4'-DDE	6.208	5.220	355.2E6	155.1E6	121.936	128.334
13)	MA Dieldrin	6.362	5.352	307.7E6	144.6E6	97.532	103.723
14)	MA Endrin	6.593	5.628	132.9E6	64701242	51.551	52.322
15)	B Endosulfa...	6.812	5.922	150.0E6	71075421	56.435	59.097
16)	A 4,4'-DDD	6.727	5.775	220.1E6	91335780	97.405	96.376
17)	MA 4,4'-DDT	7.041	6.026	255.5E6	94432157	114.449	100.805
18)	B Endrin al...	6.943	6.102	84069472	39223258	44.960	46.761
19)	B Endosulfa...	7.178	6.325	55364067	27448140	22.169	24.601
20)	A Methoxychlor	7.518	6.602	65961713	26316555	49.830	49.313
21)	B Endrin ke...	7.664	6.831	165.5E6	79018430	59.787	61.754

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080223\
Data File : PD076975.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Aug 2023 12:17
Operator : AR\AJ
Sample : 03805-09DL2 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 22:12:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

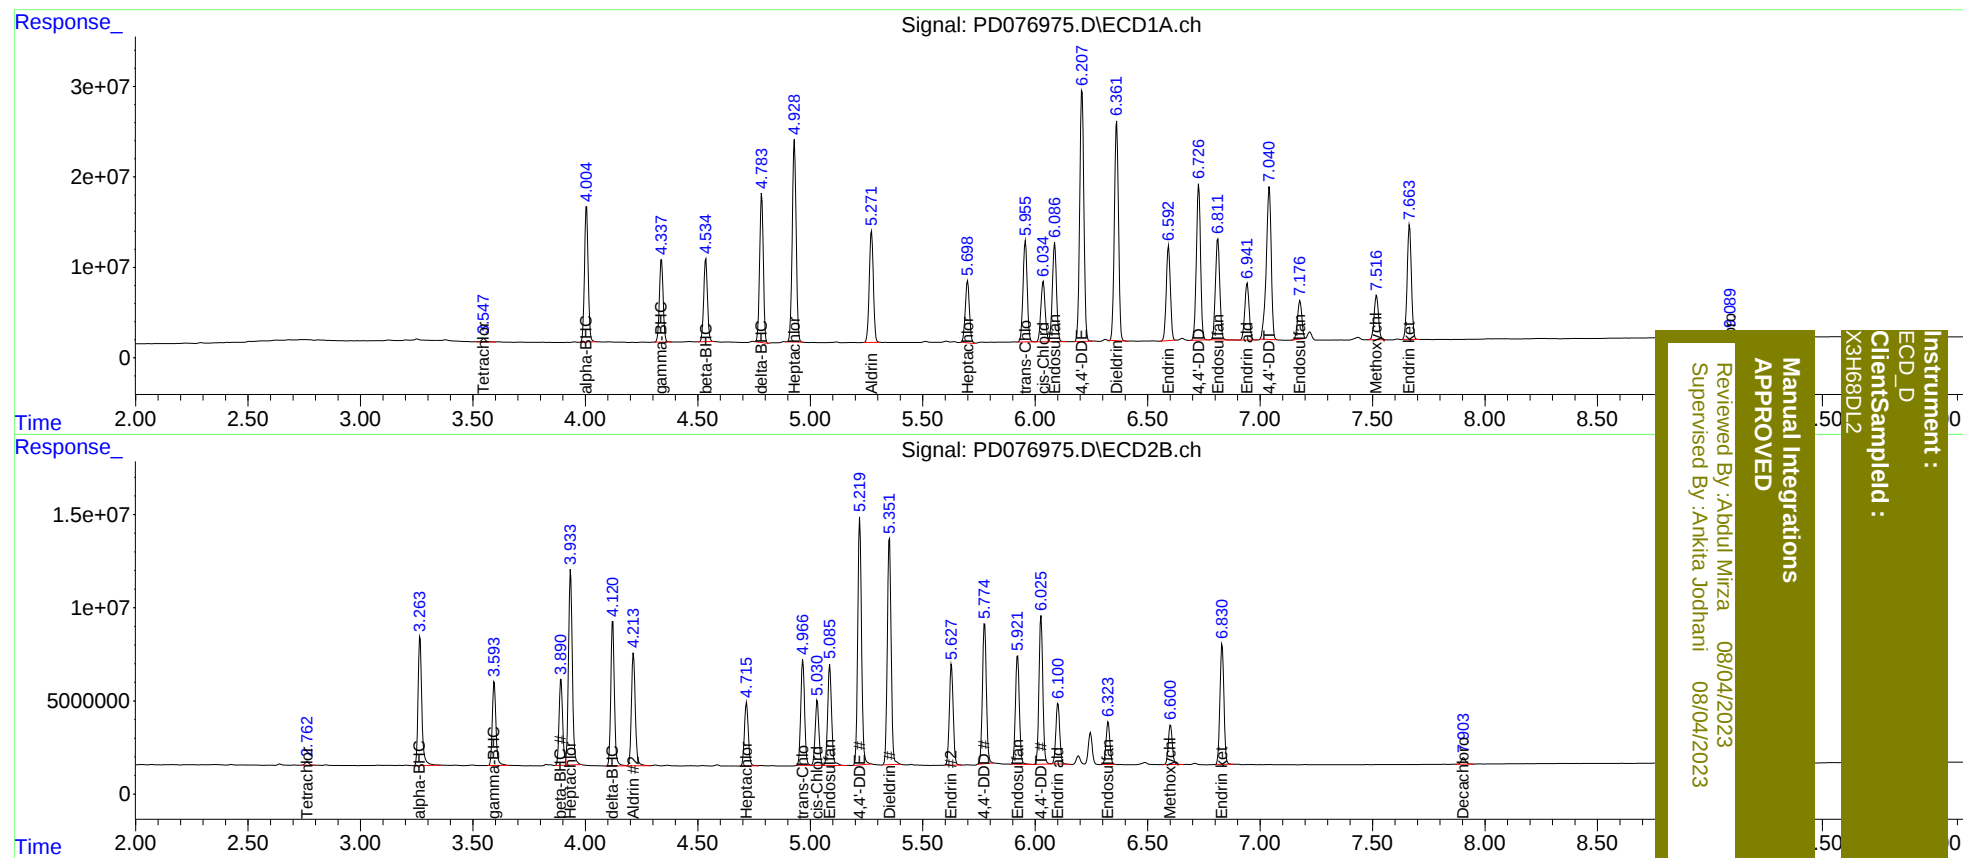

Instrument :
ECD_D
ClientSampled :
X3H68DL2

Manual Integrations
APPROVED

Reviewed By :Abdul Miza 08/04/2023
Supervised By :Ankita Jodhani 08/04/2023