

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080224\
 Data File : PD084183.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Aug 2024 10:20
 Operator : AR\AJ
 Sample : PB162453BL
 Misc : BL/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB162453BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 23:48:37 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071524.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 16 04:22:06 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.568	2.769	18330226	102.0E6	17.927	17.742
28)	SA Decachlor...	9.122	7.894	39866000	126.6E6	17.463	19.718
Target Compounds							
2)	A alpha-BHC	0.000	3.258	0	234711	N.D.	0.026 #
5)	MB Aldrin	5.292	0.000	154867	0	0.076	N.D. #
6)	B beta-BHC	0.000	3.901	0	1152630	N.D.	0.328 #
7)	B delta-BHC	4.799	4.125	821547	212185	0.452	0.026 #
10)	B gamma-Chl...	5.942f	0.000	172791	0	0.086	N.D. #
14)	MA Endrin	0.000	5.642f	0	496378	N.D.	0.075 #
18)	B Endrin al...	0.000	6.072f	0	90679	N.D.	0.018 #
24)	Chlordane-2	0.000	4.326	0	348983	N.D.	1.243 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080224\
Data File : PD084183.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Aug 2024 10:20
Operator : AR\AJ
Sample : PB162453BL
Misc : BL/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB162453BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 23:48:37 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071524.M
Quant Title : GC Extractables
QLast Update : Tue Jul 16 04:22:06 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

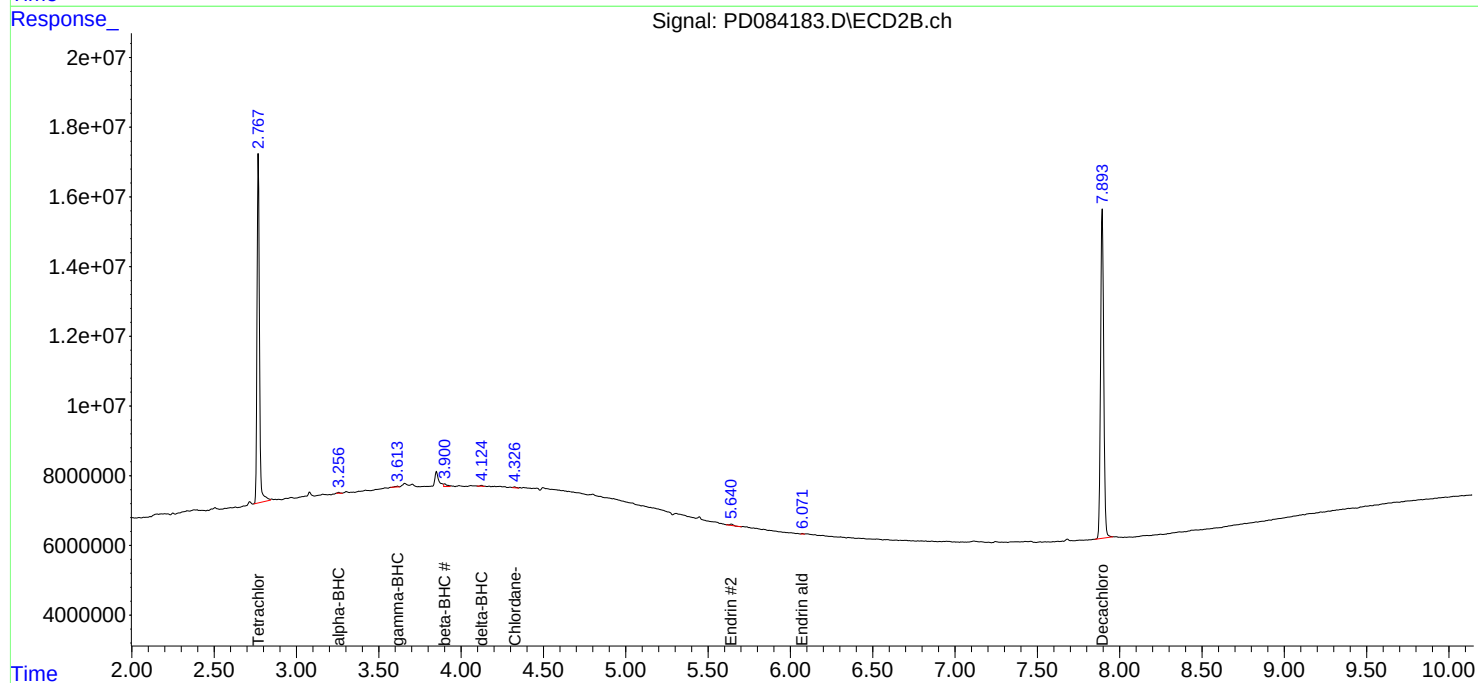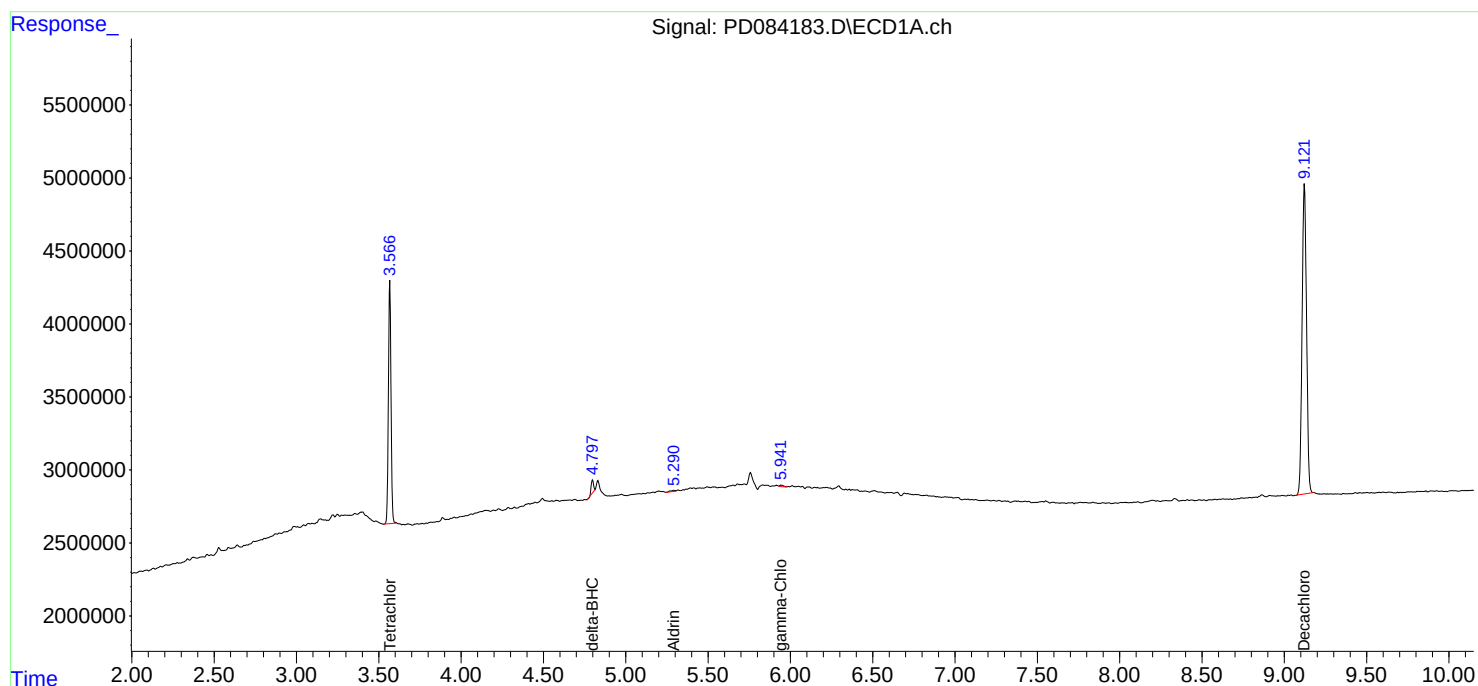


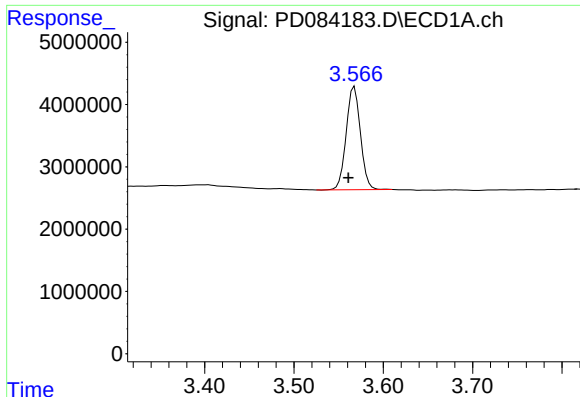

#1 Tetrachloro-m-xylene


R.T.: 3.568 min
Delta R.T.: 0.007 min
Response: 18330226
Conc: 17.93 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB162453BL

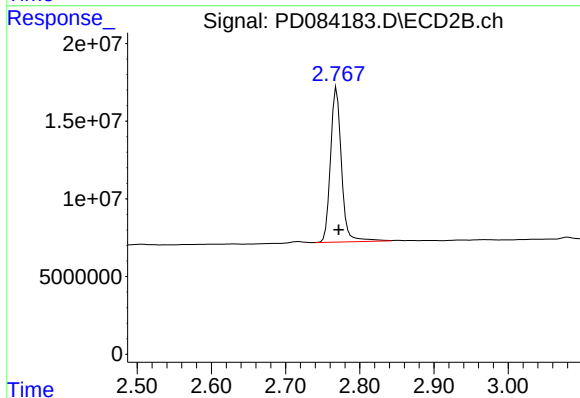


#1 Tetrachloro-m-xylene

R.T.: 2.769 min
Delta R.T.: -0.003 min
Response: 102008588
Conc: 17.74 ng/ml

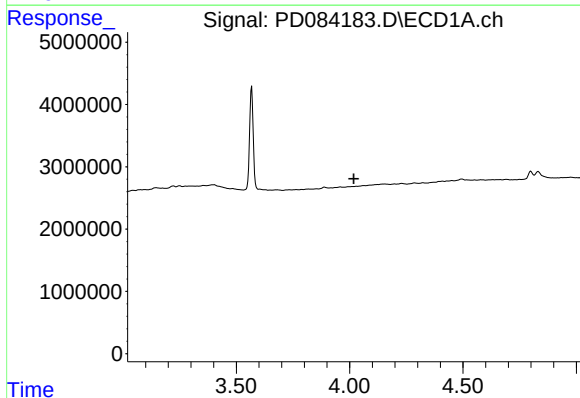


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 4.018 min
Response: 0
Conc: N.D.

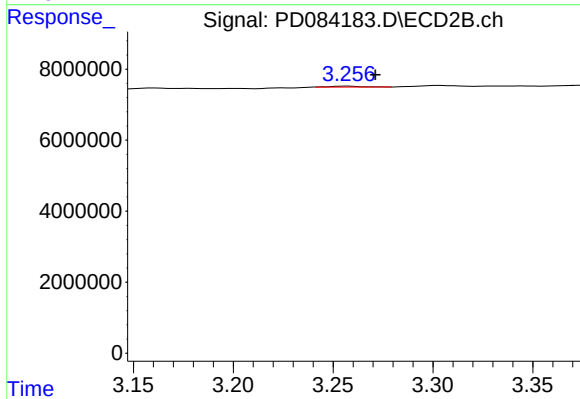

#2 alpha-BHC


R.T.: 3.258 min
Delta R.T.: -0.014 min
Response: 234711
Conc: 0.03 ng/ml

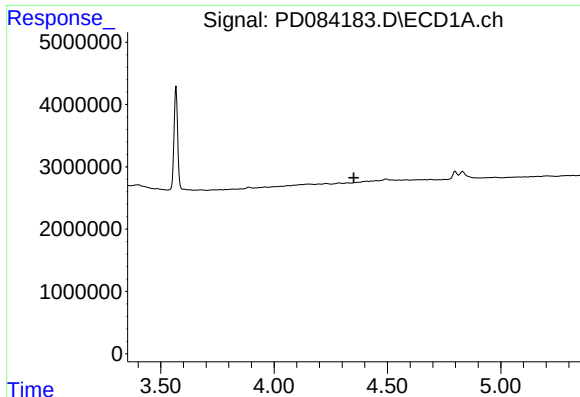

#3 gamma-BHC (Lindane)


R.T.: 4.370 min
Delta R.T.: 0.018 min
Response: -98309
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB162453BL

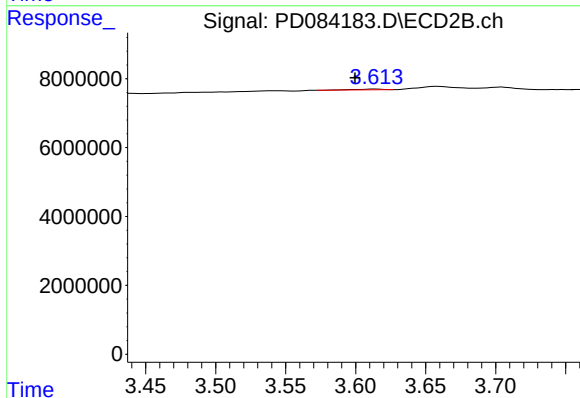


#3 gamma-BHC (Lindane)

R.T.: 3.614 min
Delta R.T.: 0.015 min
Response: 285663
Conc: 0.04 ng/ml

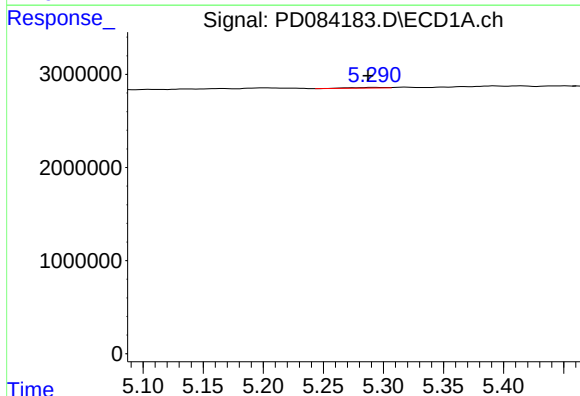


#5 Aldrin

R.T.: 5.292 min
Delta R.T.: 0.005 min
Response: 154867
Conc: 0.08 ng/ml

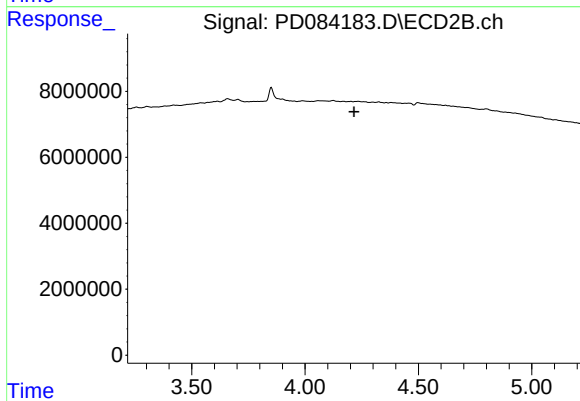

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 4.217 min
Response: 0
Conc: N.D.

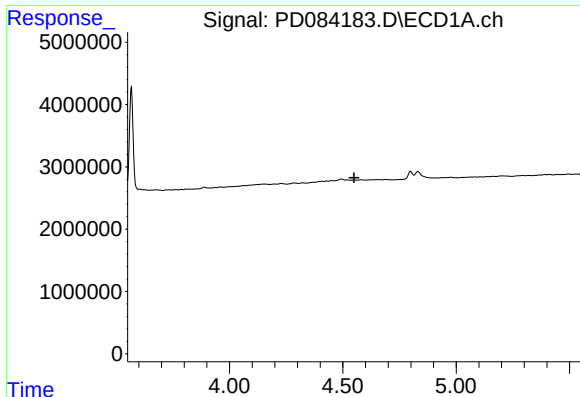

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.550 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB162453BL

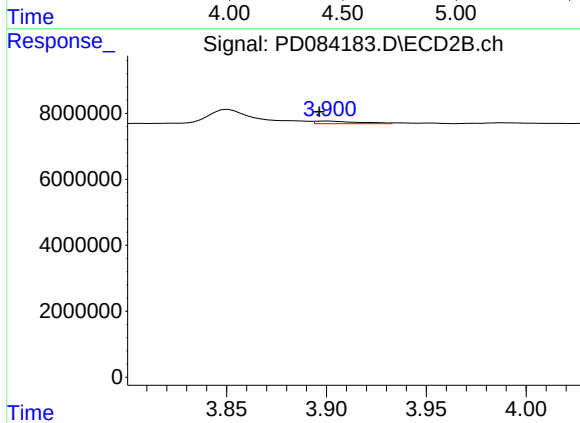


#6 beta-BHC

R.T.: 3.901 min
Delta R.T.: 0.005 min
Response: 1152630
Conc: 0.33 ng/ml

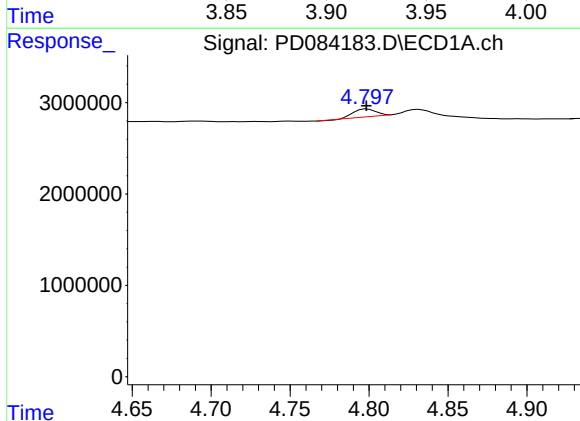


#7 delta-BHC

R.T.: 4.799 min
Delta R.T.: 0.000 min
Response: 821547
Conc: 0.45 ng/ml

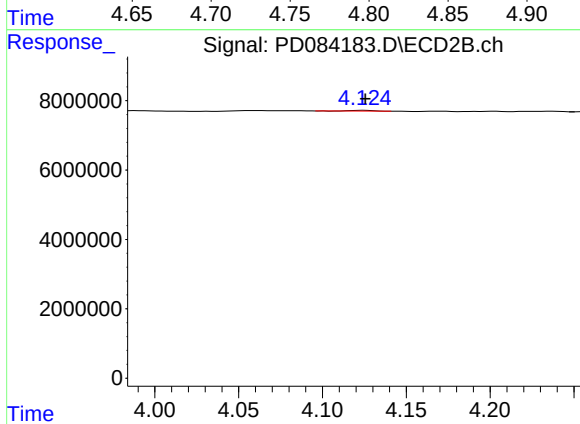

#7 delta-BHC


R.T.: 4.125 min
Delta R.T.: 0.000 min
Response: 212185
Conc: 0.03 ng/ml

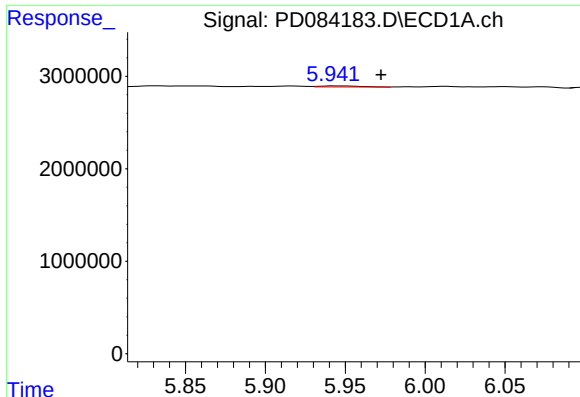

#10 gamma-Chlordane


R.T.: 5.942 min
Delta R.T.: -0.030 min
Response: 172791
Conc: 0.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB162453BL

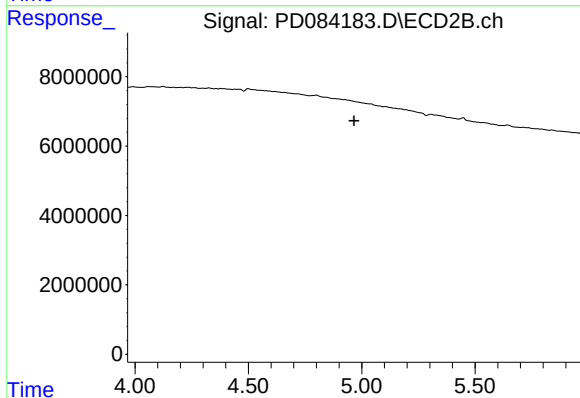


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.967 min
Response: 0
Conc: N.D.

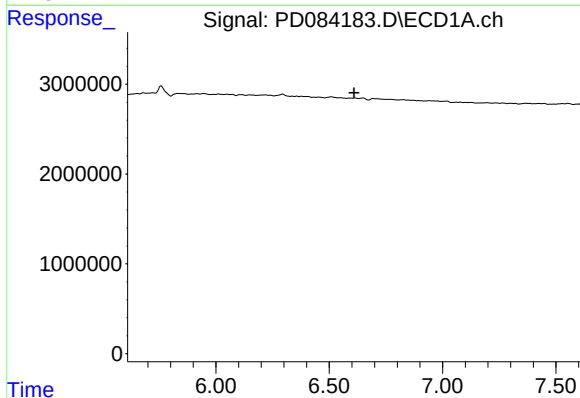


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.610 min
Response: 0
Conc: N.D.

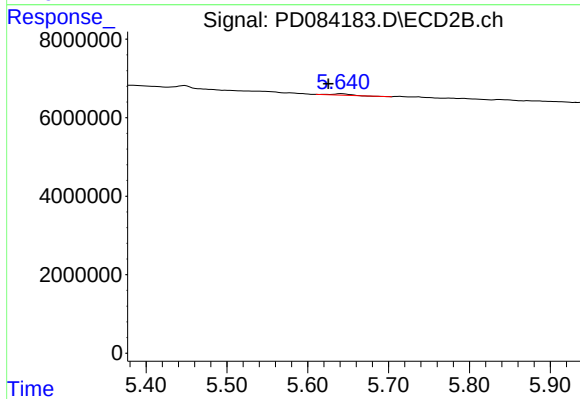

#14 Endrin


R.T.: 5.642 min
Delta R.T.: 0.016 min
Response: 496378
Conc: 0.08 ng/ml

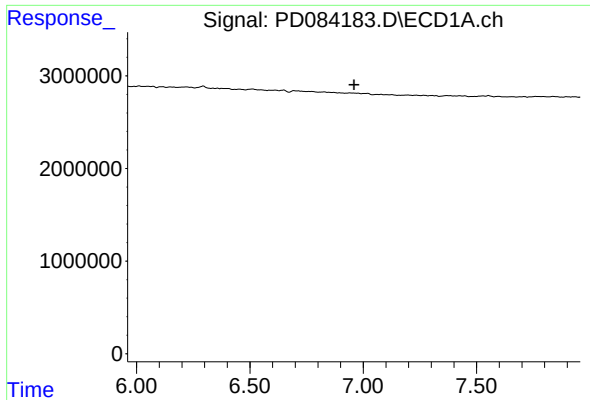

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.960 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB162453BL

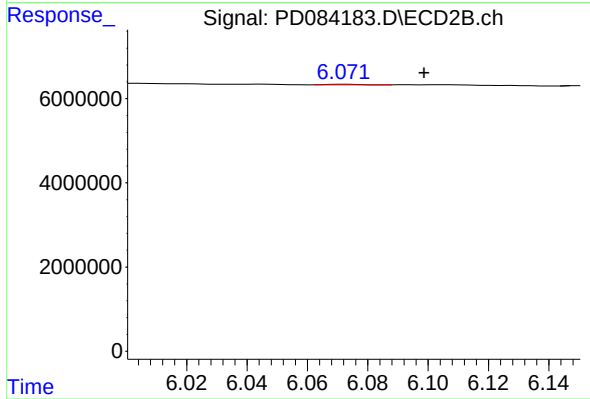


#18 Endrin aldehyde

R.T.: 6.072 min
Delta R.T.: -0.026 min
Response: 90679
Conc: 0.02 ng/ml

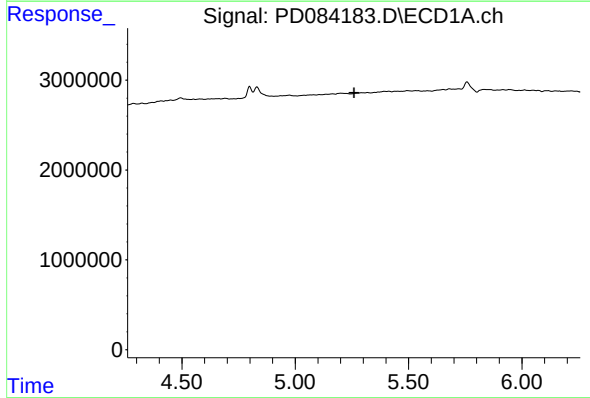


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 5.260 min
Response: 0
Conc: N.D.

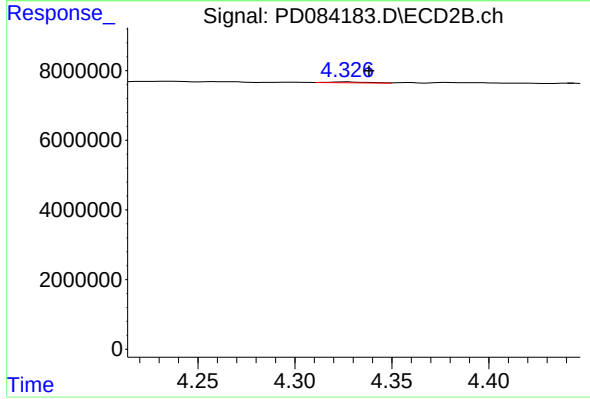

#24 Chlordane-2


R.T.: 4.326 min
Delta R.T.: -0.012 min
Response: 348983
Conc: 1.24 ng/ml

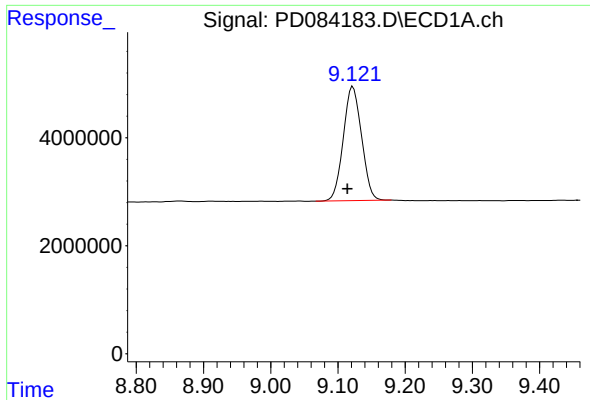

#28 Decachlorobiphenyl

R.T.: 9.122 min
Delta R.T.: 0.008 min
Response: 39866000
Conc: 17.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB162453BL

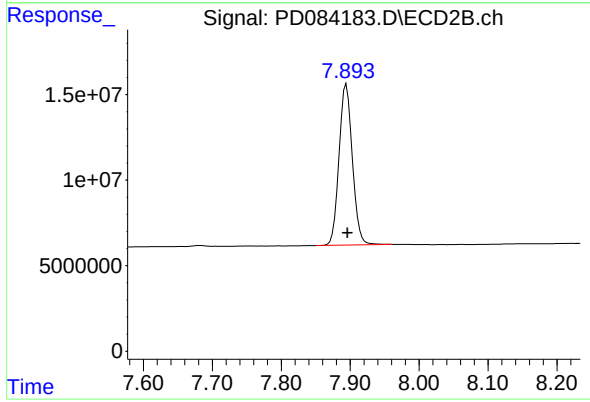

#28 Decachlorobiphenyl

R.T.: 7.894 min
Delta R.T.: -0.001 min
Response: 126629737
Conc: 19.72 ng/ml