

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080224\
 Data File : PD084183.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Aug 2024 10:20
 Operator : AR\AJ
 Sample : PB162453BL
 Misc : BL/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB162453BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 23:48:37 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071524.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 16 04:22:06 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.568	2.769	18330226	102.0E6	17.927	17.742
28) SA Decachlor...	9.122	7.894	39866000	126.6E6	17.463	19.718

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080224\
Data File : PD084183.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Aug 2024 10:20
Operator : AR\AJ
Sample : PB162453BL
Misc : BL/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB162453BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 23:48:37 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071524.M
Quant Title : GC Extractables
QLast Update : Tue Jul 16 04:22:06 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

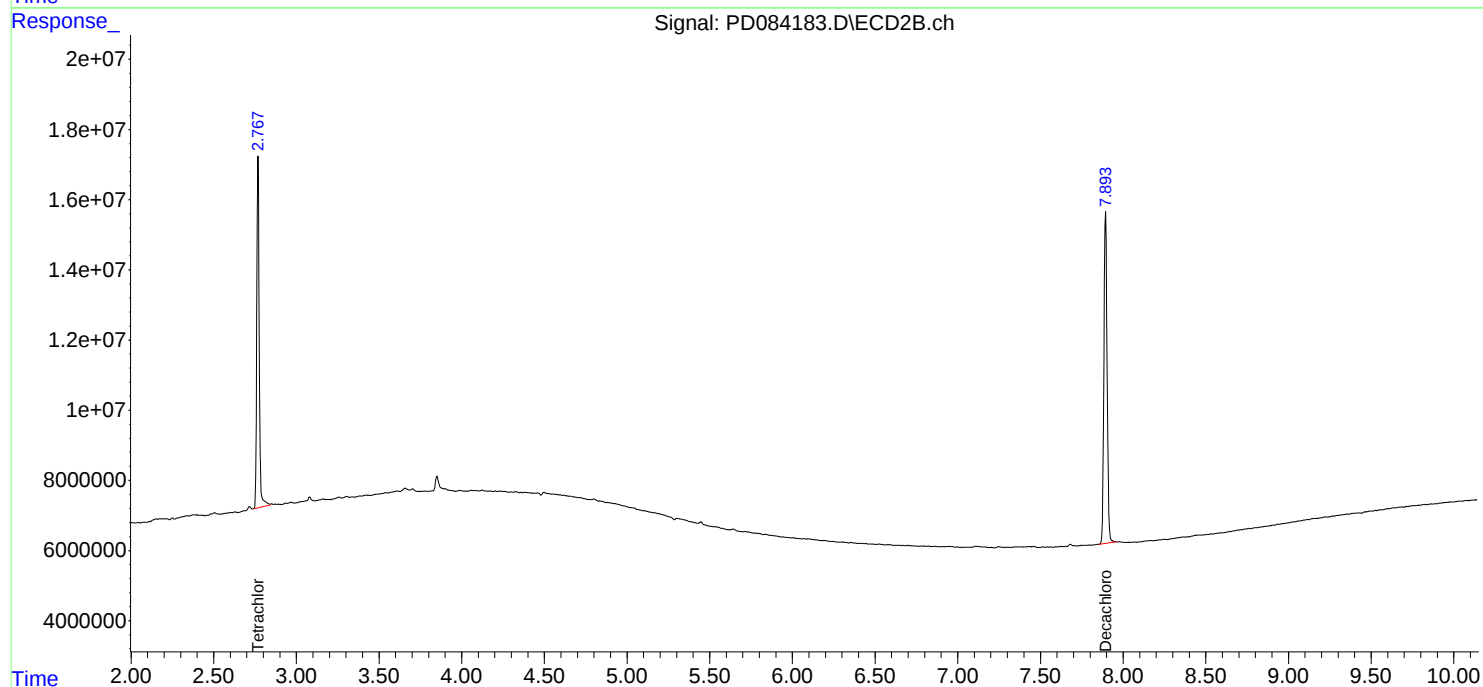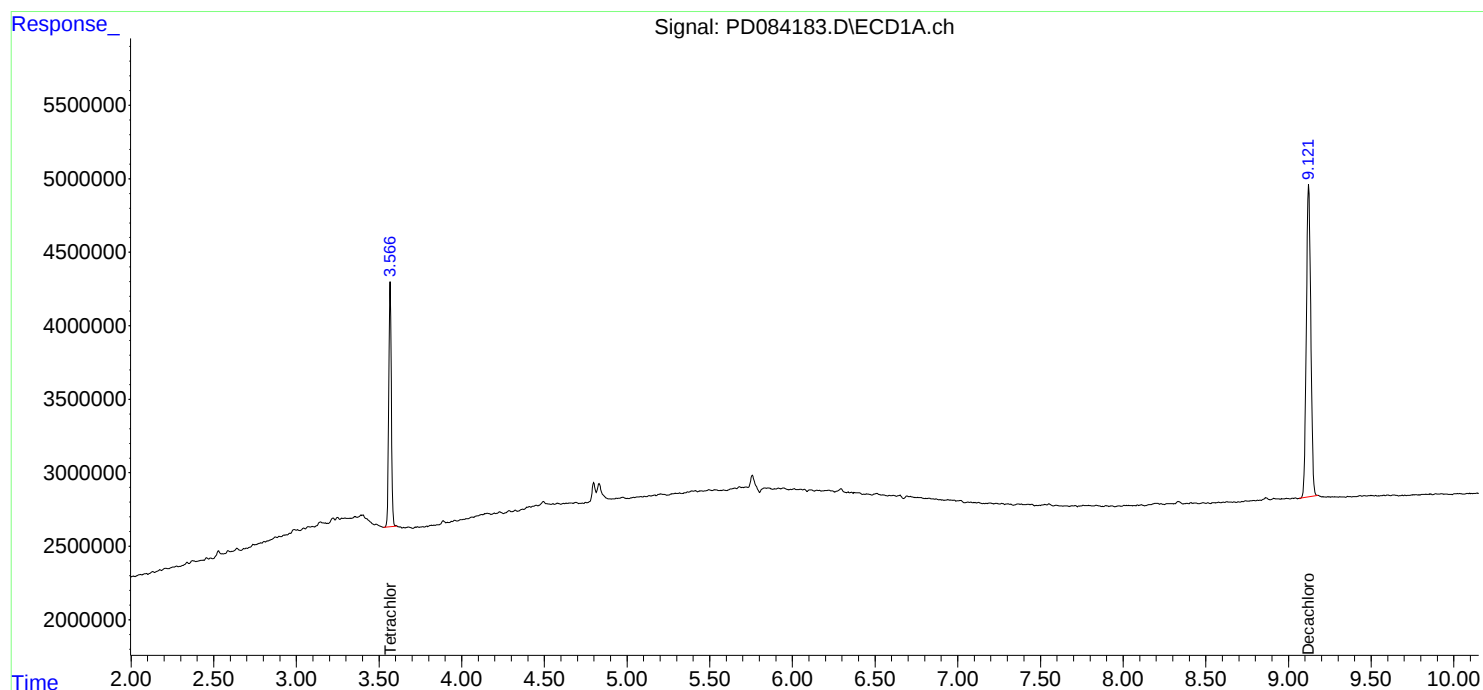


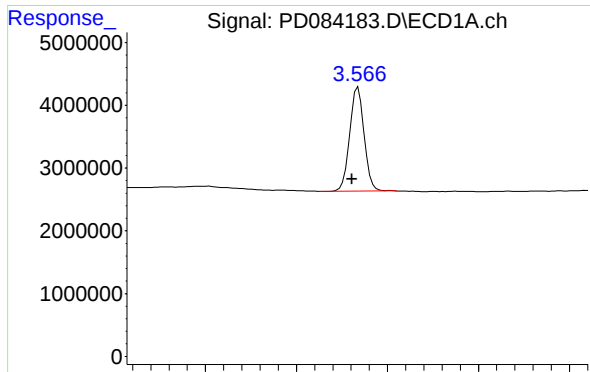

#1 Tetrachloro-m-xylene


R.T.: 3.568 min
Delta R.T.: 0.007 min
Response: 18330226
Conc: 17.93 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB162453BL

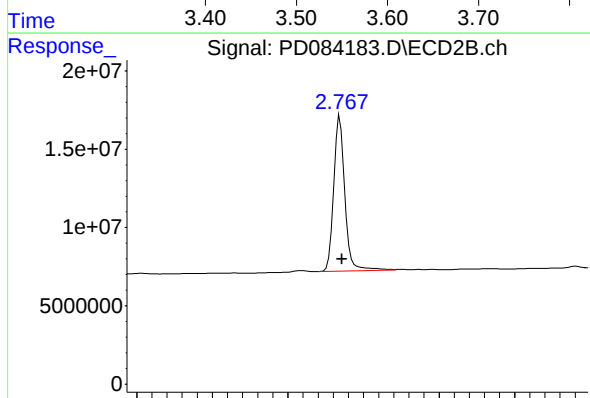


#1 Tetrachloro-m-xylene

R.T.: 2.769 min
Delta R.T.: -0.003 min
Response: 102008588
Conc: 17.74 ng/ml

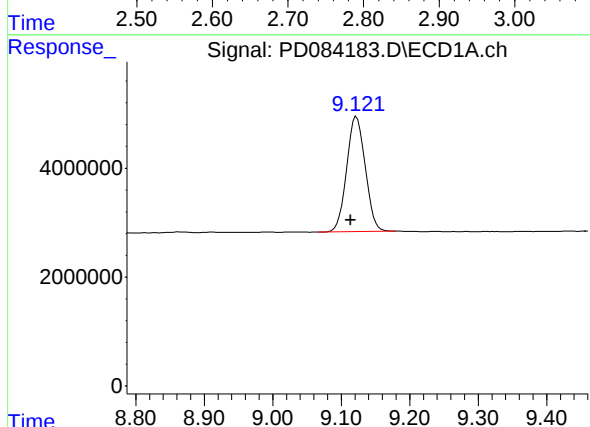

#28 Decachlorobiphenyl

R.T.: 9.122 min
Delta R.T.: 0.008 min
Response: 39866000
Conc: 17.46 ng/ml

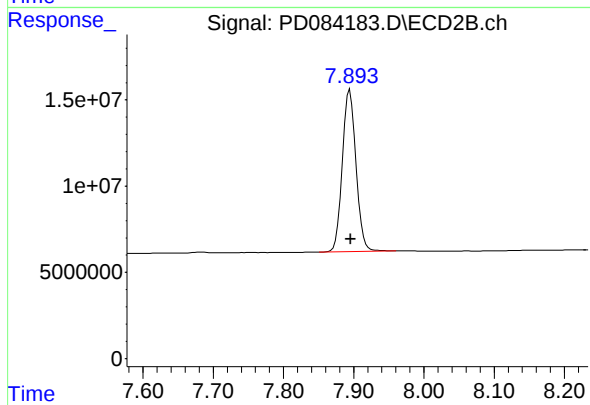

#28 Decachlorobiphenyl

R.T.: 7.894 min
Delta R.T.: -0.001 min
Response: 126629737
Conc: 19.72 ng/ml