

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080318\
 Data File : PD048750.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Aug 2018 18:53
 Operator : AJ\SJ
 Sample : J4265-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AB0

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 03 23:11:16 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072818CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 28 05:19:54 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.371	3.968	23520774	305.7E6	17.072	15.894
27)	SA Decachlor...	8.067	8.992	57587524	618.8E6	35.551	34.470
Target Compounds							
9)	A Endosulfan I	0.000	6.127f	0	6000993	N.D.	0.265
10)	B trans-Chl...	0.000	6.127f	0	6000993	N.D.	0.241
11)	B cis-Chlor...	0.000	6.127	0	6000993	N.D.	0.250


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080318\
Data File : PD048750.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Aug 2018 18:53
Operator : AJ\SJ
Sample : J4265-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C0AB0

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 03 23:11:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072818CLP.M
Quant Title : GC Extractables
QLast Update : Sat Jul 28 05:19:54 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

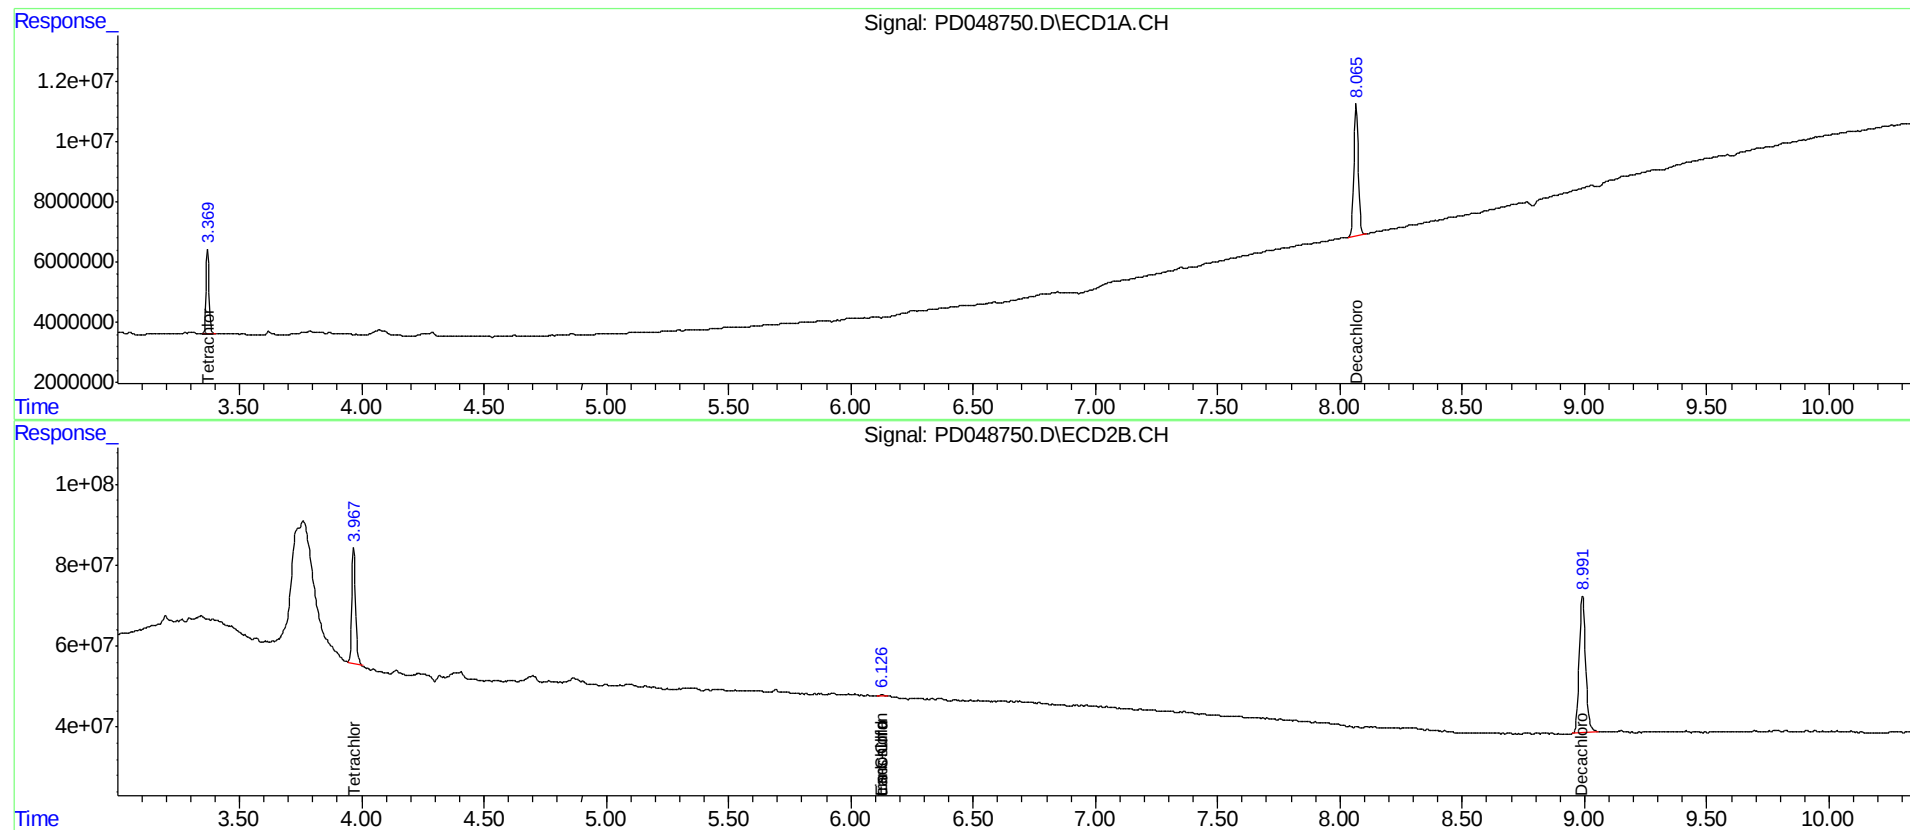


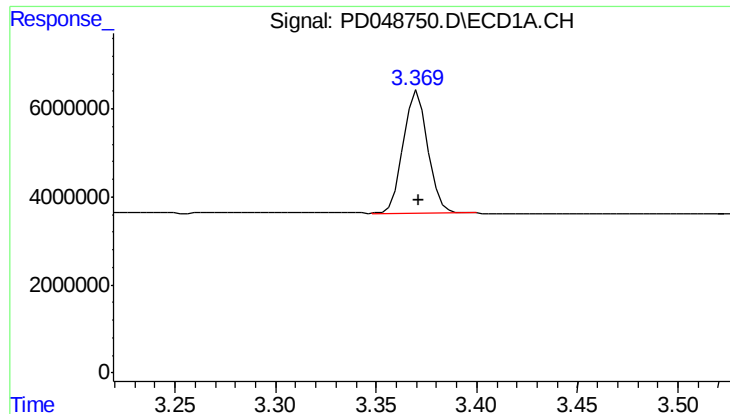

#1 Tetrachloro-m-xylene


R.T.: 3.371 min
Delta R.T.: 0.000 min
Response: 23520774
Conc: 17.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AB0

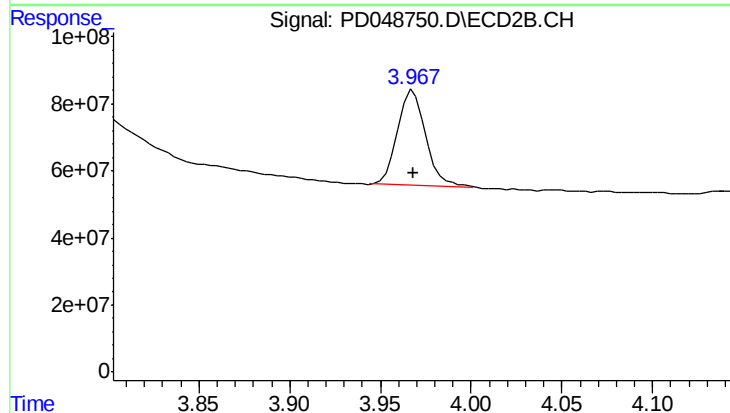


#1 Tetrachloro-m-xylene

R.T.: 3.968 min
Delta R.T.: 0.000 min
Response: 305725844
Conc: 15.89 ng/ml

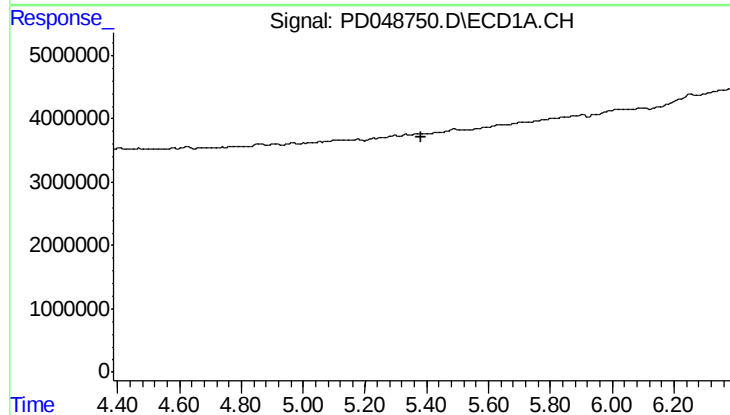


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.383 min
Response: 0
Conc: N.D.

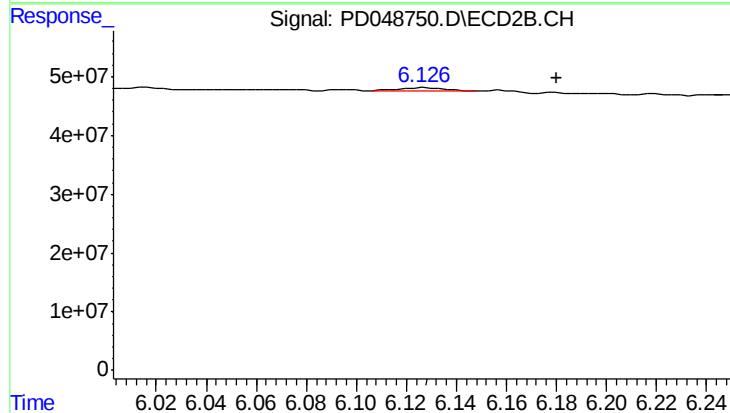

#9 Endosulfan I


R.T.: 6.127 min
Delta R.T.: -0.053 min
Response: 6000993
Conc: 0.27 ng/ml

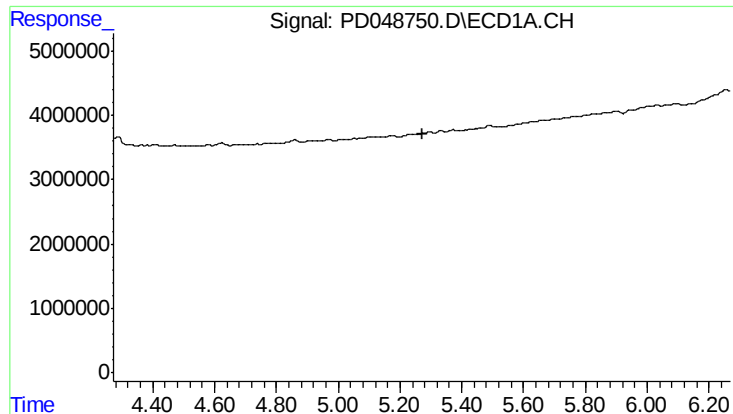

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.272 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0AB0

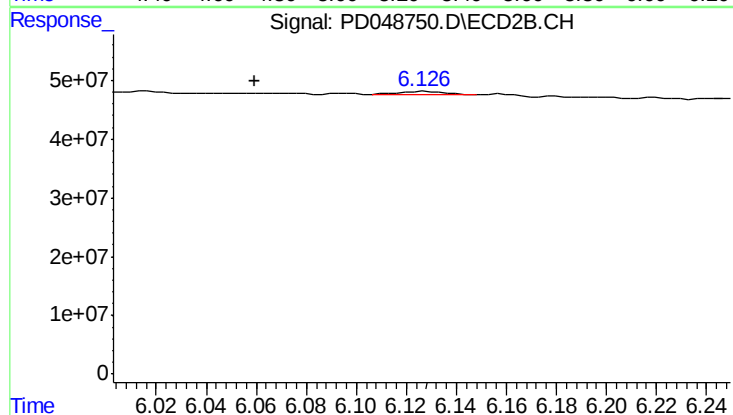


#10 trans-Chlordane

R.T.: 6.127 min
Delta R.T.: 0.068 min
Response: 6000993
Conc: 0.24 ng/ml

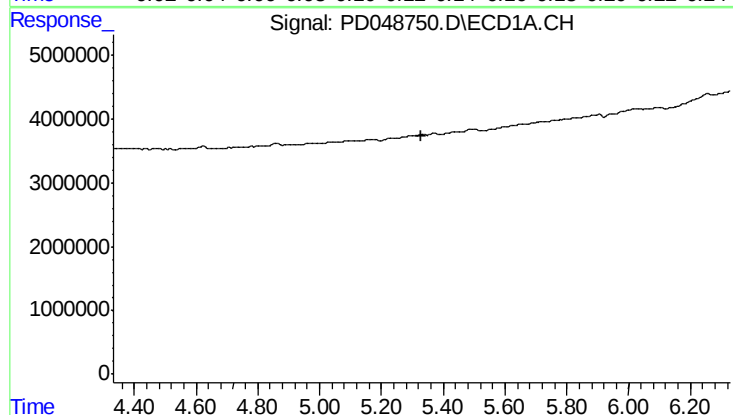


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.330 min
Response: 0
Conc: N.D.

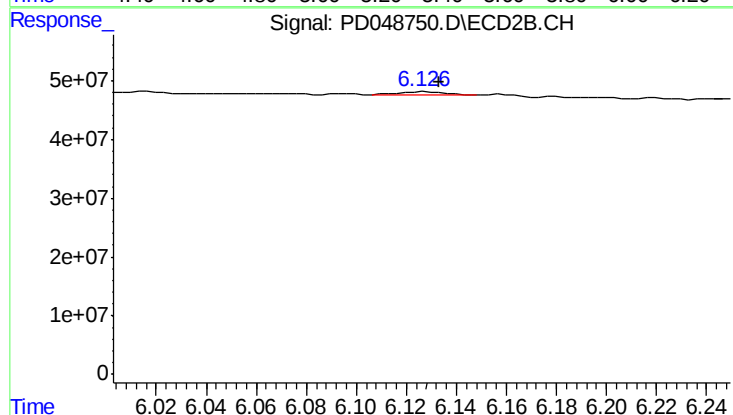

#11 cis-Chlordane


R.T.: 6.127 min
Delta R.T.: -0.006 min
Response: 6000993
Conc: 0.25 ng/ml

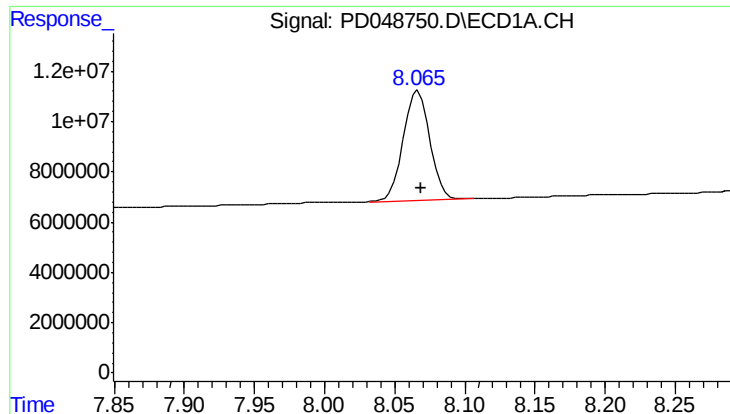

#27 Decachlorobiphenyl

R.T.: 8.067 min
Delta R.T.: -0.002 min
Response: 57587524
Conc: 35.55 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AB0

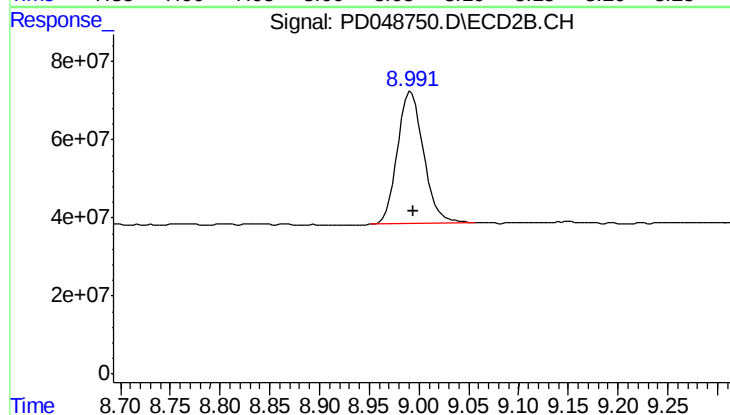

#27 Decachlorobiphenyl

R.T.: 8.992 min
Delta R.T.: -0.002 min
Response: 618759215
Conc: 34.47 ng/ml