

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080320\
 Data File : PD058852.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Aug 2020 10:16
 Operator : DD\AJ
 Sample : PB130654BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PBLK54

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 04 01:28:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073120CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 30 03:06:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.216	3.868	32966586	50620906	21.130	22.644
27)	SA Decachlor...	7.854	8.865	60187245	76546689	37.473	37.170
Target Compounds							
14)	MA Endrin	0.000	6.589f	0	1840698	N.D.	0.980
15)	B Endosulfa...	0.000	6.769	0	151835	N.D.	<MDL


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080320\
Data File : PD058852.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Aug 2020 10:16
Operator : DD\AJ
Sample : PB130654BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PBLK54

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 04 01:28:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073120CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 30 03:06:29 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

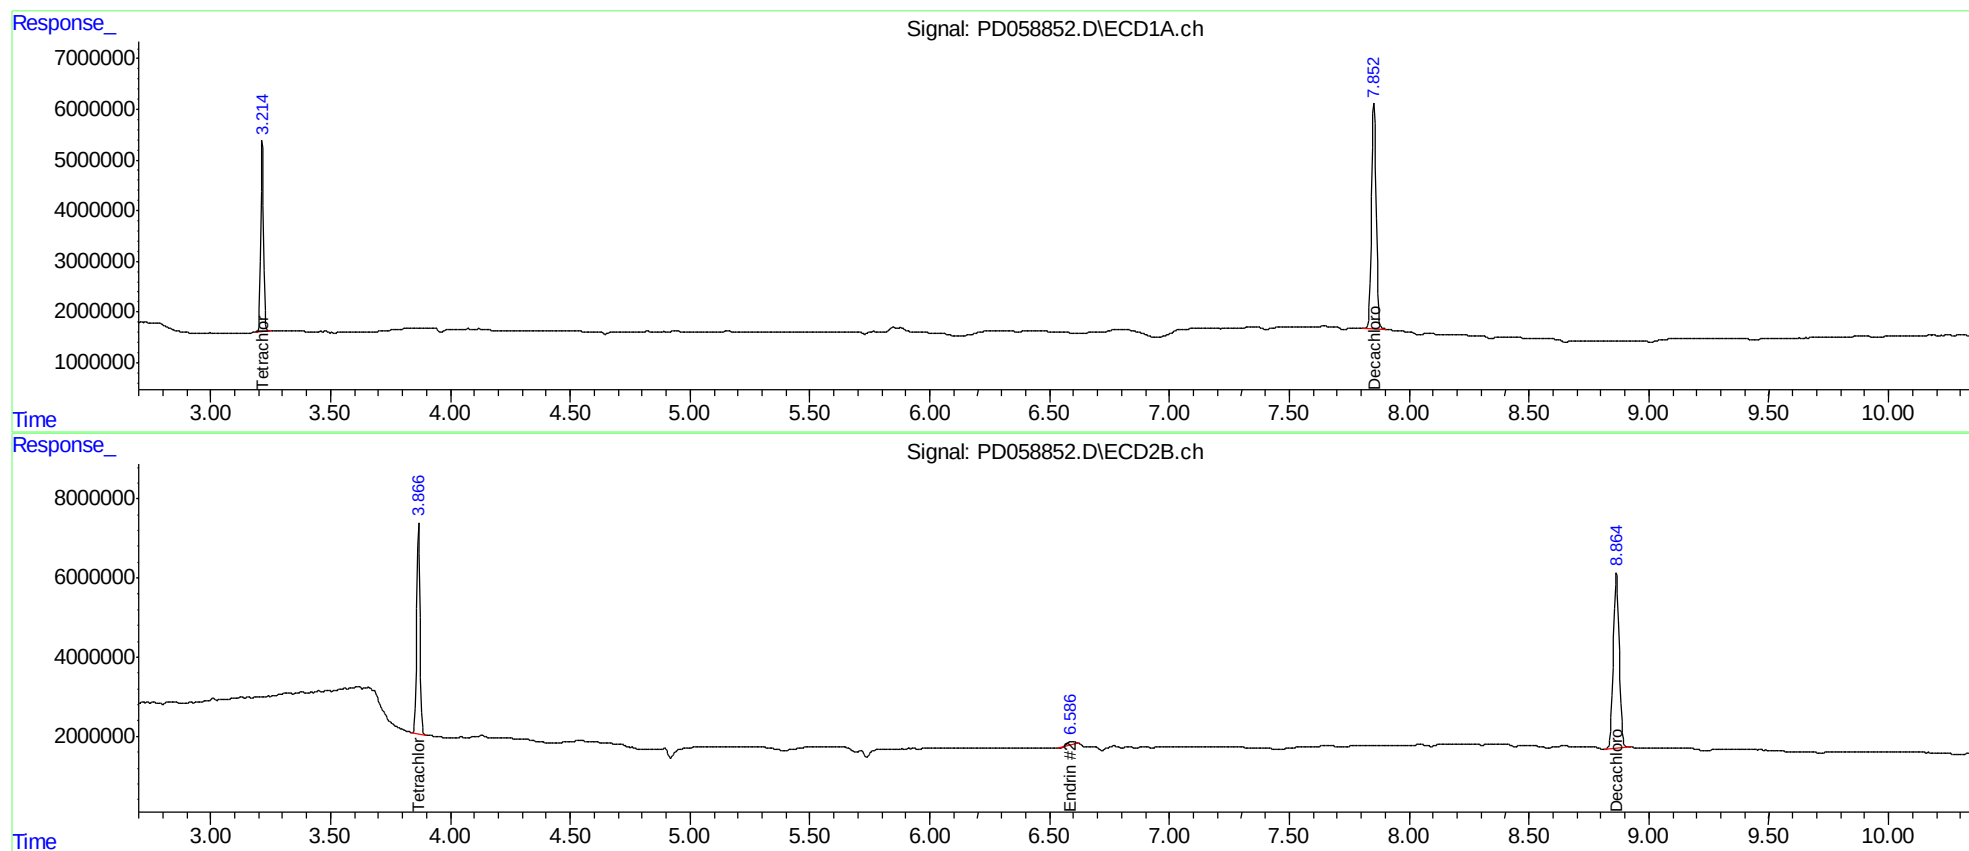


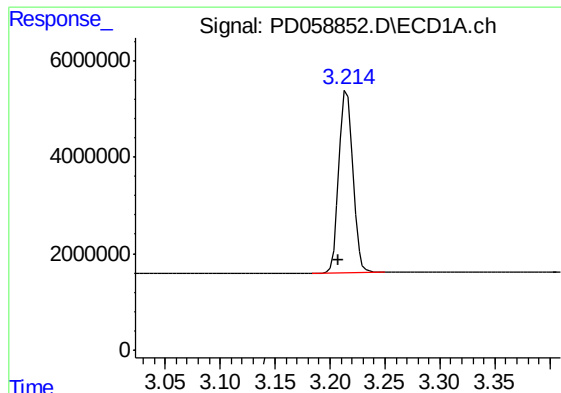

#1 Tetrachloro-m-xylene


R.T.: 3.216 min
Delta R.T.: 0.008 min
Response: 32966586
Conc: 21.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK54

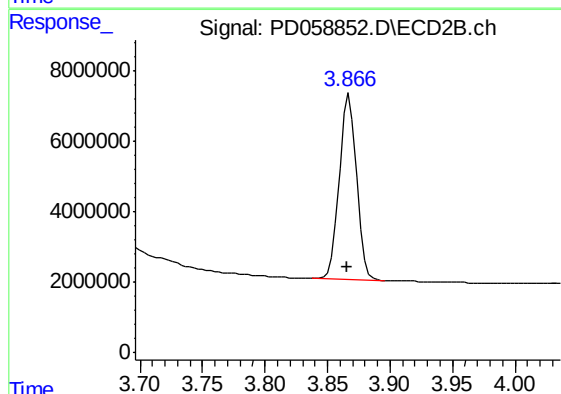


#1 Tetrachloro-m-xylene

R.T.: 3.868 min
Delta R.T.: 0.002 min
Response: 50620906
Conc: 22.64 ng/ml

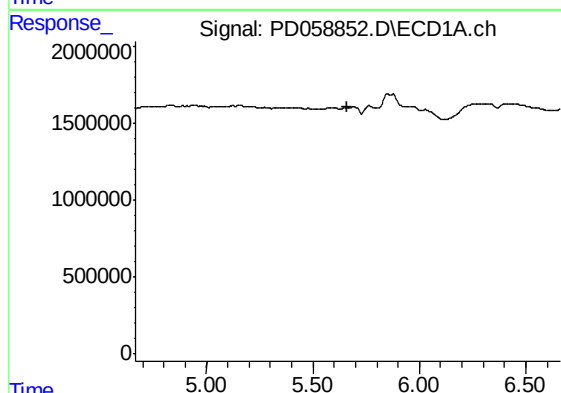


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 5.663 min
Response: 0
Conc: N.D.

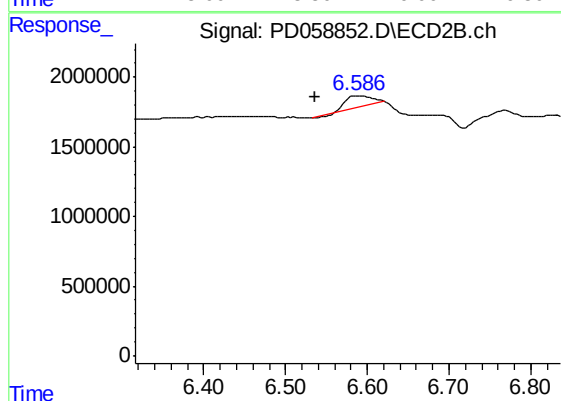

#14 Endrin


R.T.: 6.589 min
Delta R.T.: 0.053 min
Response: 1840698
Conc: 0.98 ng/ml

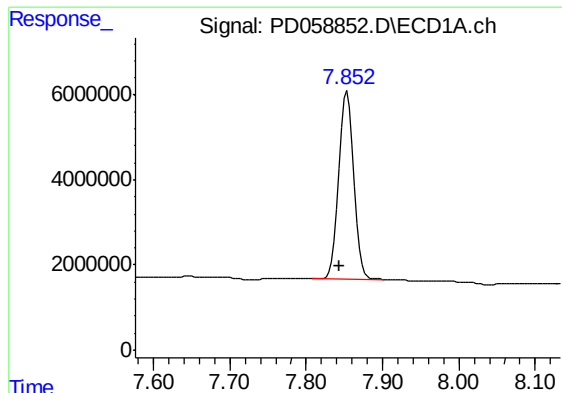

#27 Decachlorobiphenyl

R.T.: 7.854 min
Delta R.T.: 0.011 min
Response: 60187245
Conc: 37.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK54

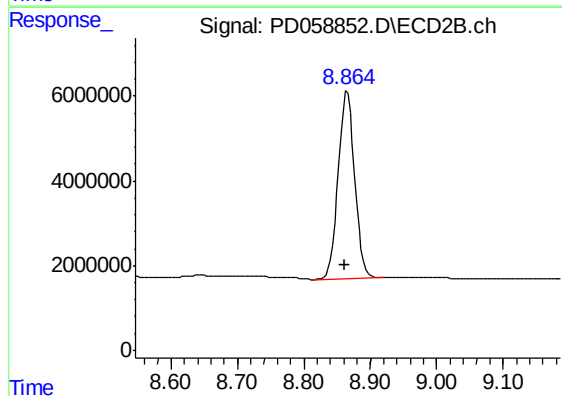

#27 Decachlorobiphenyl

R.T.: 8.865 min
Delta R.T.: 0.004 min
Response: 76546689
Conc: 37.17 ng/ml