

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080323\
 Data File : PD076992.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Aug 2023 13:05
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 03 14:02:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 13:58:43 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	2.762	56360934	38067984	25.257	25.261
28)	SA Decachlor...	9.084	7.904	67822287	34990858	26.746	26.308
Target Compounds							
23)	Chlordane-1	4.708	3.759	26752878	12245498	253.038	254.129
24)	Chlordane-2	5.239	4.335	30645052	14275614	265.730	262.307
25)	Chlordane-3	5.952	4.966	114.7E6	39855403	245.227	249.223
26)	Chlordane-4	6.034	5.029	141.9E6	38924521	249.893	244.165
27)	Chlordane-5	6.886	5.925	23134253	14566565	248.771	254.507



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080323\
Data File : PD076992.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Aug 2023 13:05
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 03 14:02:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 13:58:43 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

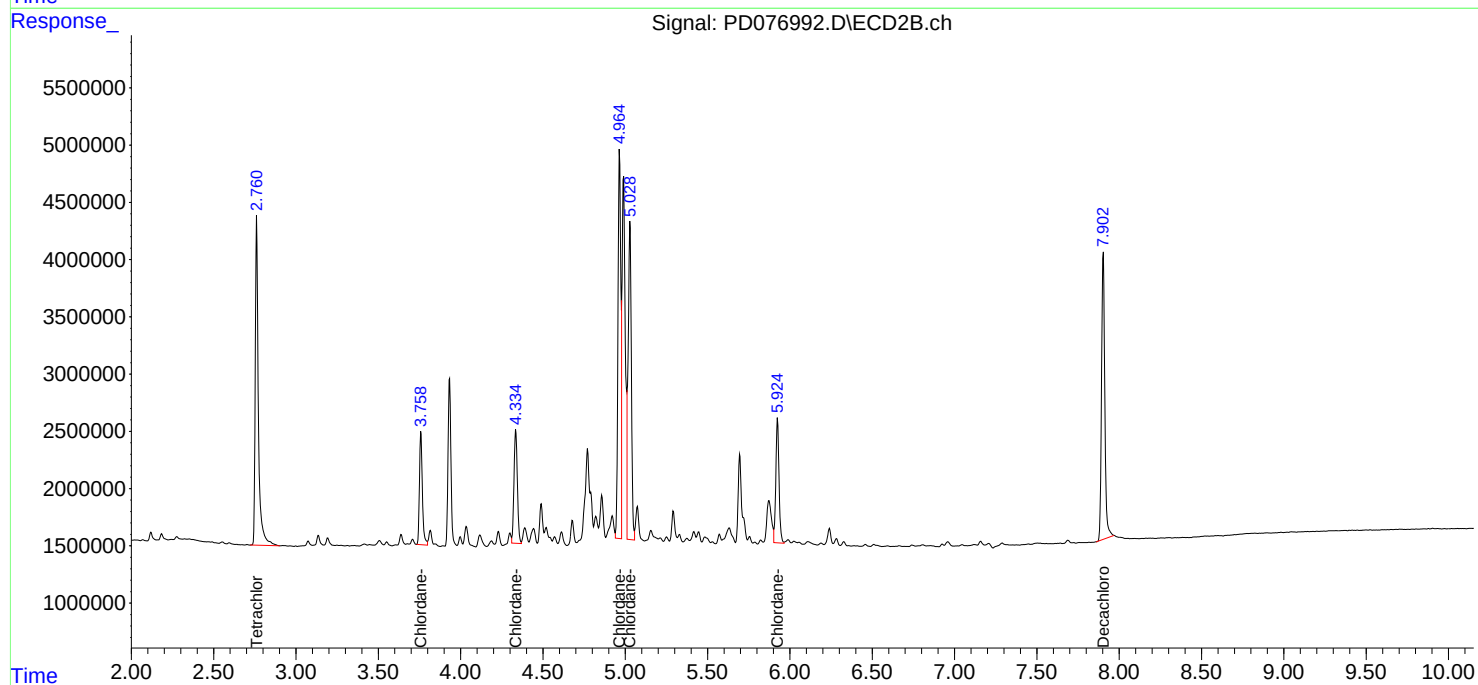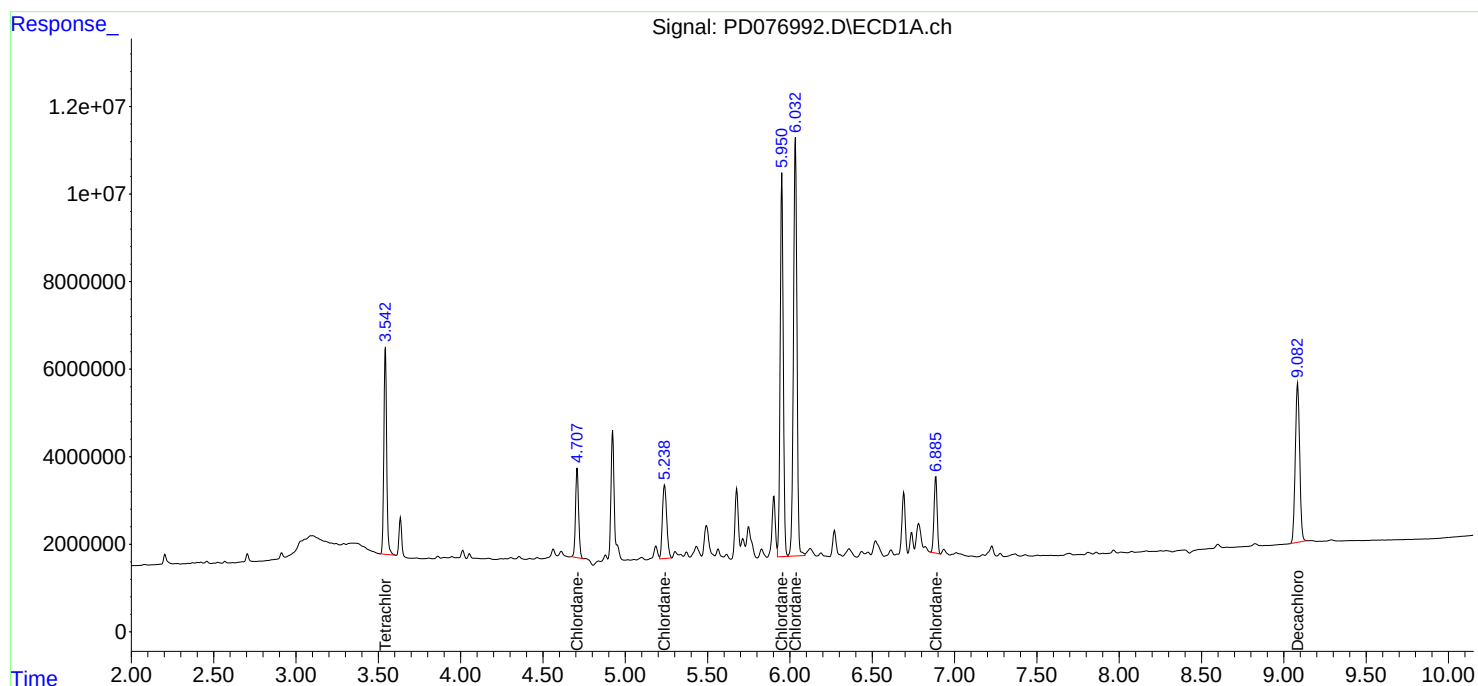


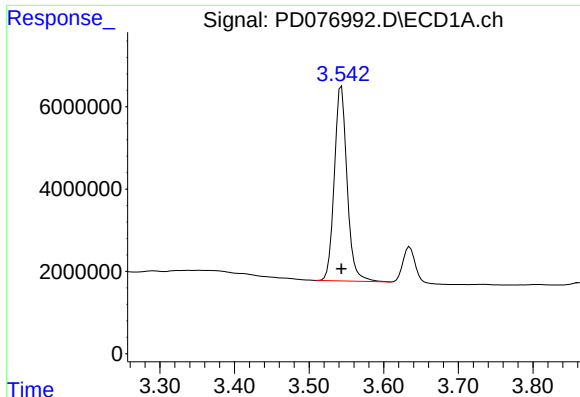

#1 Tetrachloro-m-xylene


R.T.: 3.543 min
Delta R.T.: 0.000 min
Response: 56360934
Conc: 25.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

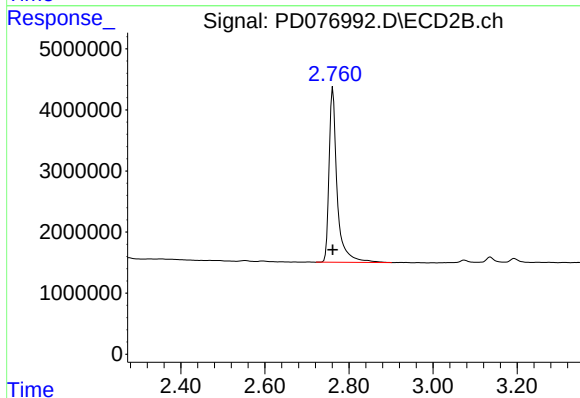


#1 Tetrachloro-m-xylene

R.T.: 2.762 min
Delta R.T.: 0.000 min
Response: 38067984
Conc: 25.26 ng/ml

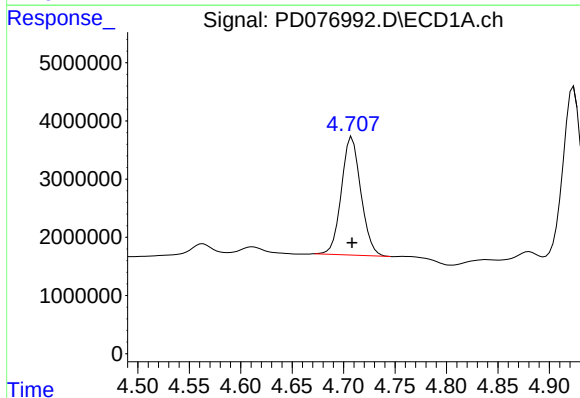


#23 Chlordane-1

R.T.: 4.708 min
Delta R.T.: 0.000 min
Response: 26752878
Conc: 253.04 ng/ml

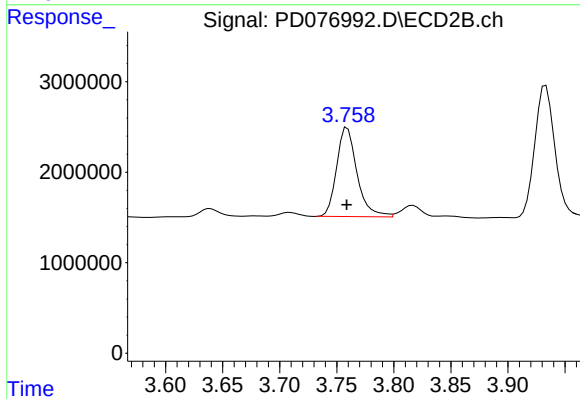

#23 Chlordane-1


R.T.: 3.759 min
Delta R.T.: 0.000 min
Response: 12245498
Conc: 254.13 ng/ml

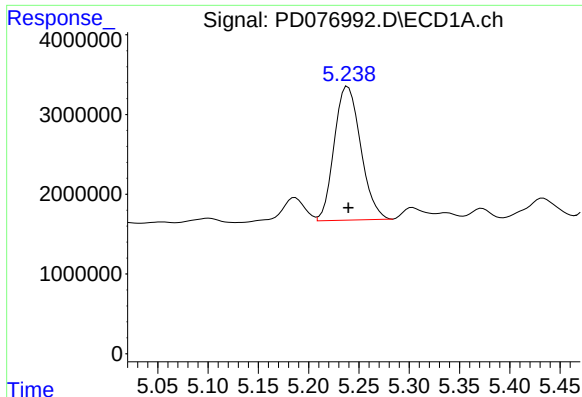

#24 Chlordane-2


R.T.: 5.239 min
Delta R.T.: 0.000 min
Response: 30645052
Conc: 265.73 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

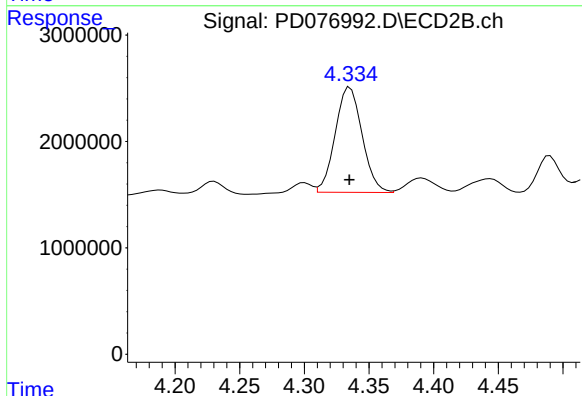


#24 Chlordane-2

R.T.: 4.335 min
Delta R.T.: 0.000 min
Response: 14275614
Conc: 262.31 ng/ml

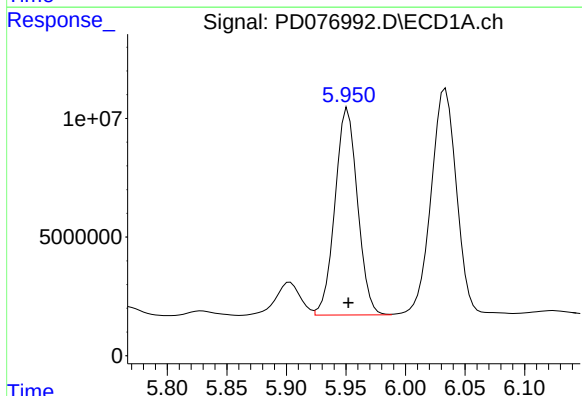


#25 Chlordane-3

R.T.: 5.952 min
Delta R.T.: 0.000 min
Response: 114659291
Conc: 245.23 ng/ml

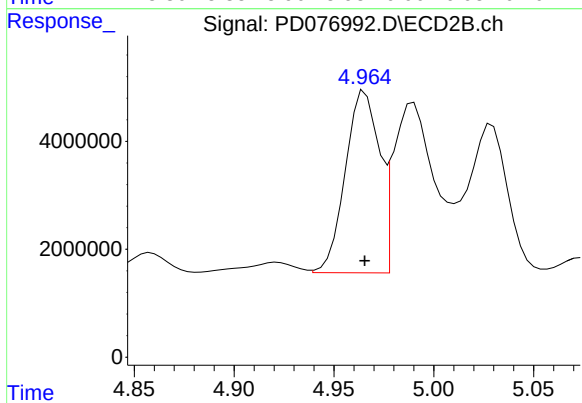

#25 Chlordane-3


R.T.: 4.966 min
Delta R.T.: 0.000 min
Response: 39855403
Conc: 249.22 ng/ml

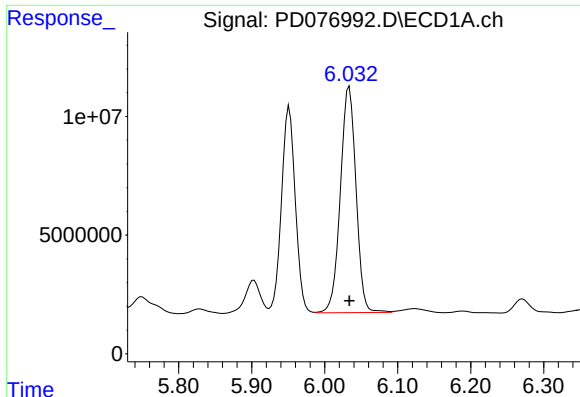

#26 Chlordane-4


R.T.: 6.034 min
Delta R.T.: 0.000 min
Response: 141865799
Conc: 249.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

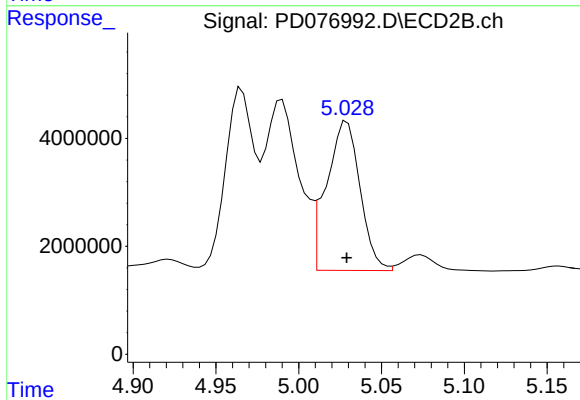


#26 Chlordane-4

R.T.: 5.029 min
Delta R.T.: 0.000 min
Response: 38924521
Conc: 244.17 ng/ml

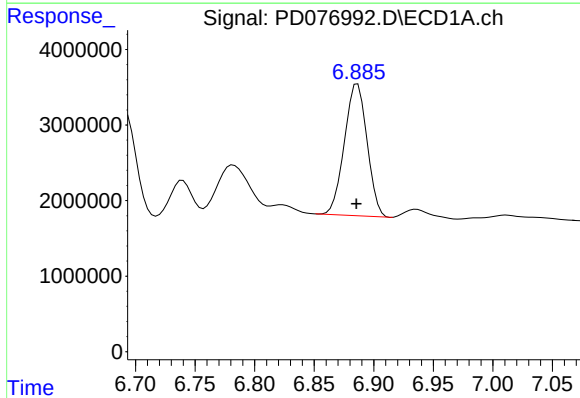


#27 Chlordane-5

R.T.: 6.886 min
Delta R.T.: 0.000 min
Response: 23134253
Conc: 248.77 ng/ml

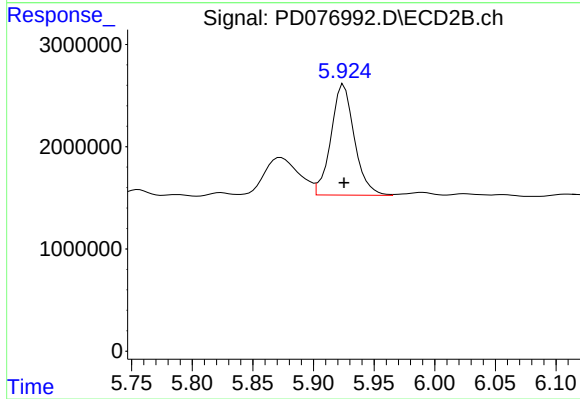

#27 Chlordane-5


R.T.: 5.925 min
Delta R.T.: 0.000 min
Response: 14566565
Conc: 254.51 ng/ml

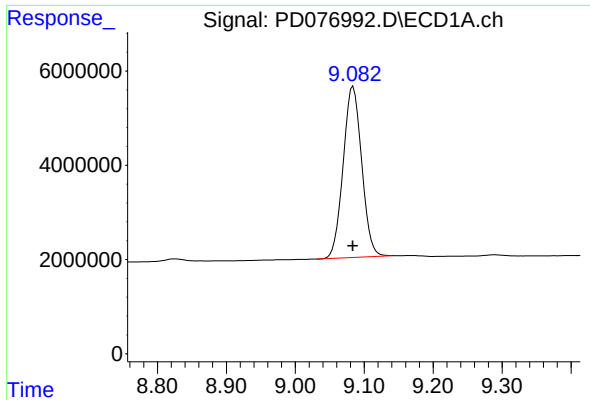

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: 0.000 min
Response: 67822287
Conc: 26.75 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

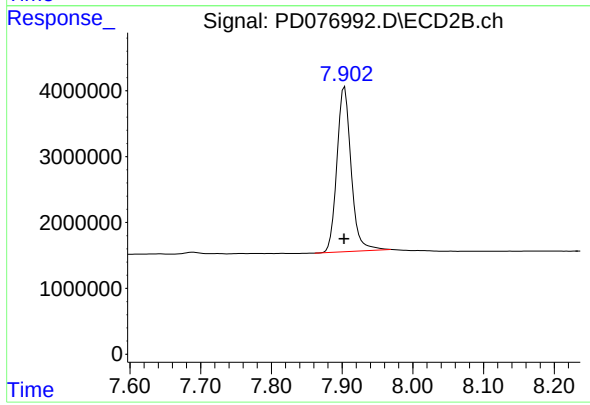

#28 Decachlorobiphenyl

R.T.: 7.904 min
Delta R.T.: 0.000 min
Response: 34990858
Conc: 26.31 ng/ml