

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080323\
 Data File : PD076993.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Aug 2023 13:19
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 03 14:02:18 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 13:58:43 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	2.762	11798993	7567100	5.288	5.021
28)	SA Decachlor...	9.084	7.902	15043183	7980804	5.932	6.000
Target Compounds							
23)	Chlordane-1	4.707	3.759	5696899	2706216	53.883	56.162
24)	Chlordane-2	5.238	4.335	7161572	3199263	62.100	58.785
25)	Chlordane-3	5.951	4.965	23368871	8241885	49.980	51.538
26)	Chlordane-4	6.033	5.028	29317930	8221976	51.643	51.575
27)	Chlordane-5	6.885	5.924	4351744	3309972	46.796	57.832



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080323\
Data File : PD076993.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Aug 2023 13:19
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 03 14:02:18 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 13:58:43 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

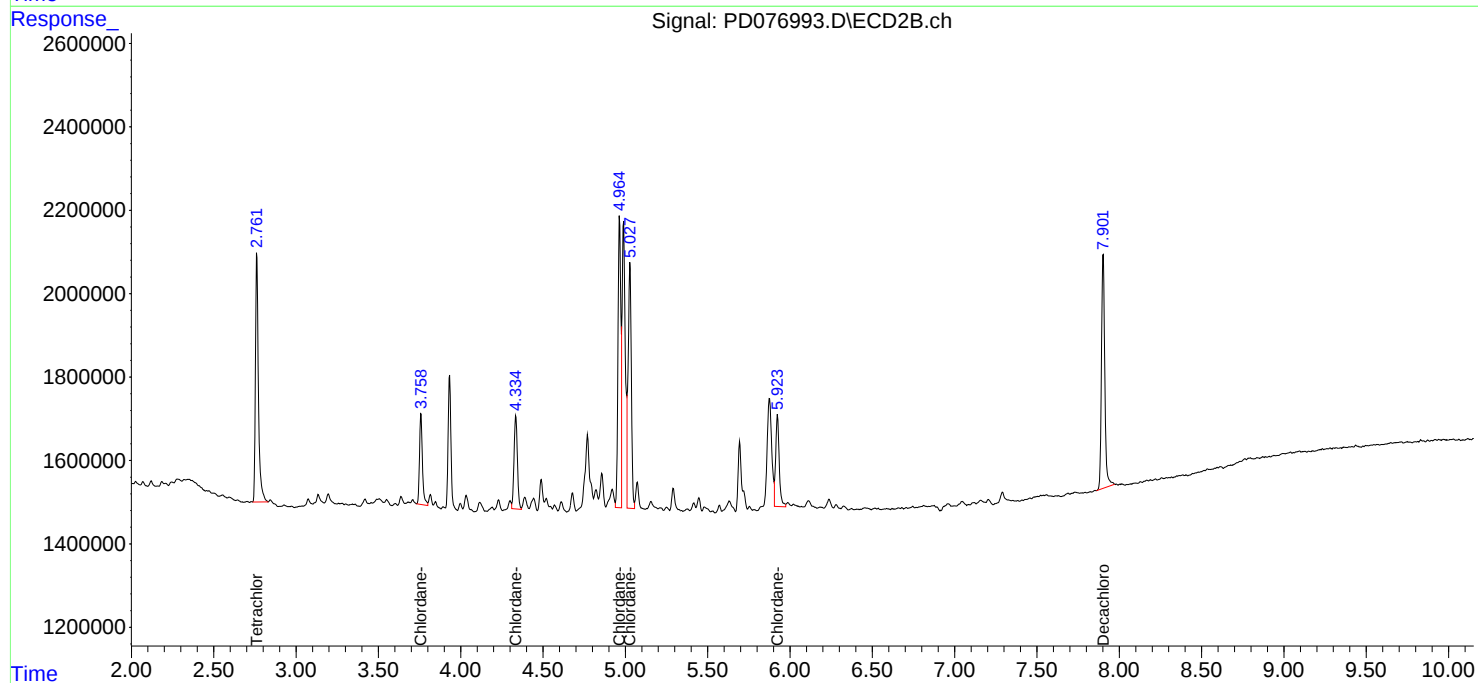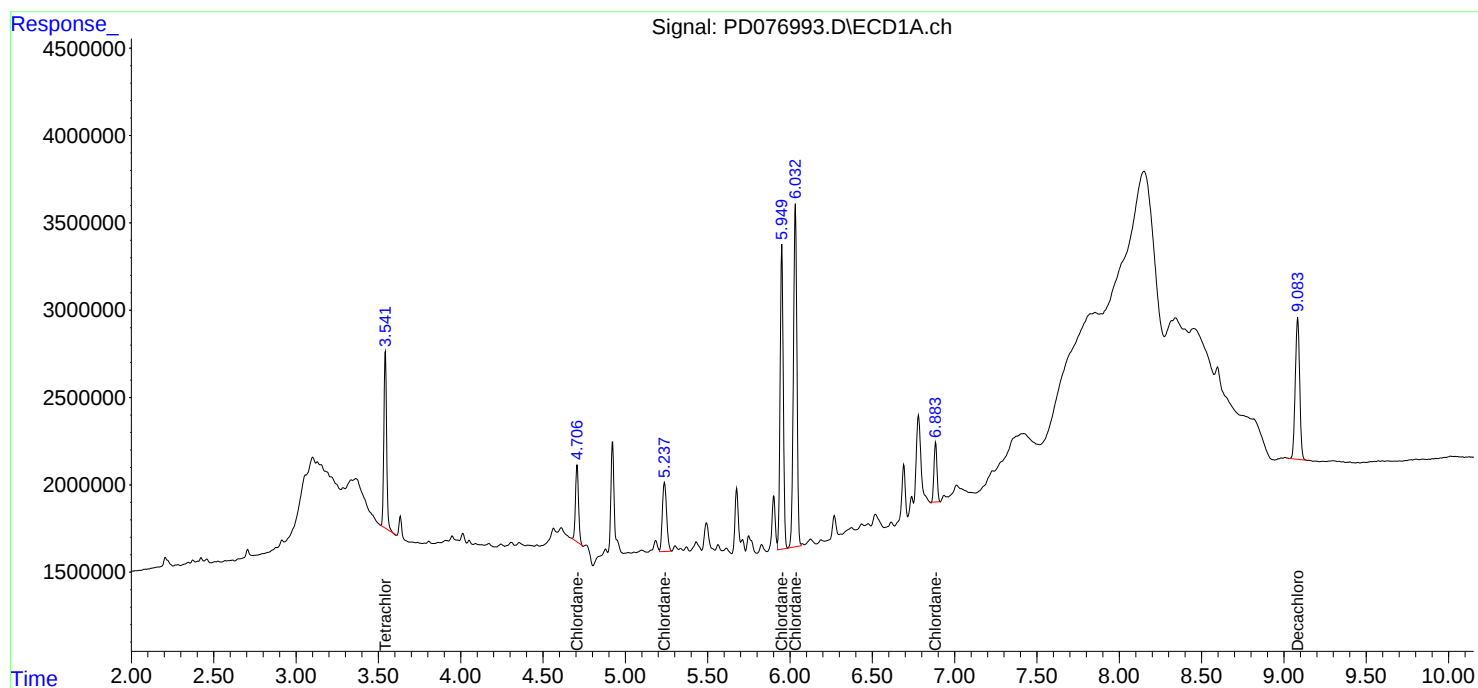


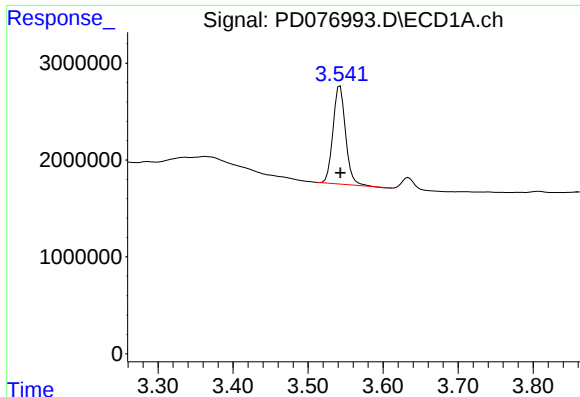

#1 Tetrachloro-m-xylene


R.T.: 3.543 min
Delta R.T.: 0.000 min
Response: 11798993
Conc: 5.29 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

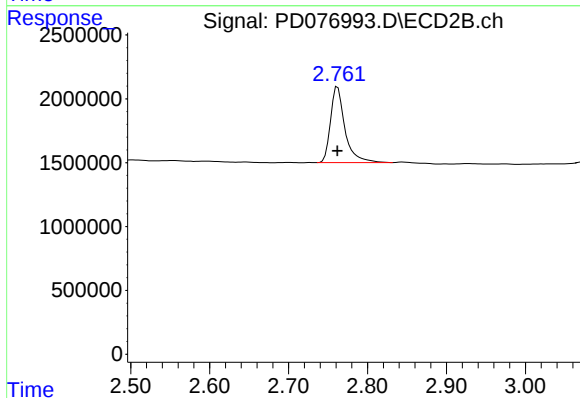


#1 Tetrachloro-m-xylene

R.T.: 2.762 min
Delta R.T.: 0.000 min
Response: 7567100
Conc: 5.02 ng/ml

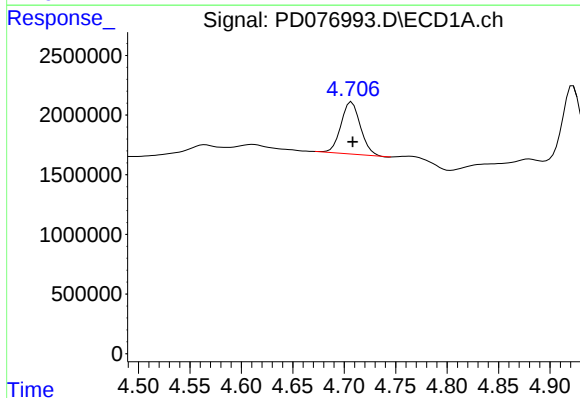


#23 Chlordane-1

R.T.: 4.707 min
Delta R.T.: 0.000 min
Response: 5696899
Conc: 53.88 ng/ml

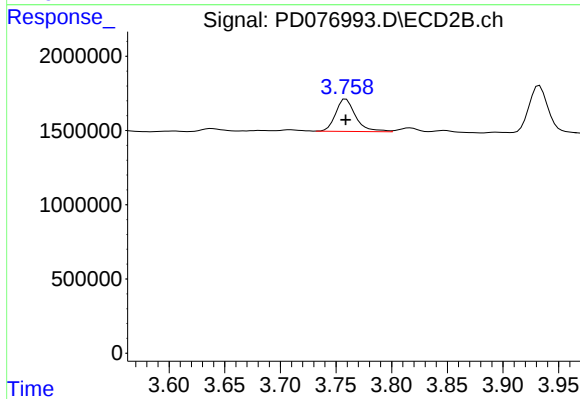

#23 Chlordane-1


R.T.: 3.759 min
Delta R.T.: 0.000 min
Response: 2706216
Conc: 56.16 ng/ml

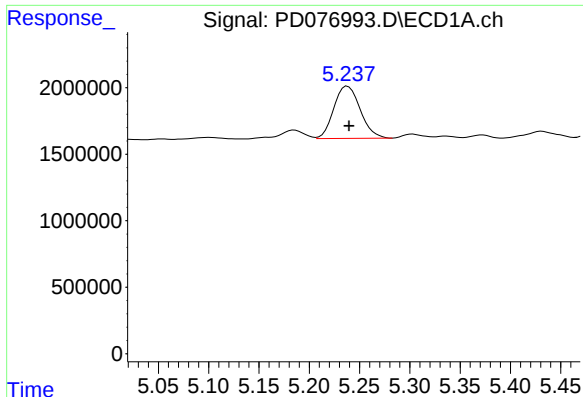

#24 Chlordane-2


R.T.: 5.238 min
Delta R.T.: -0.001 min
Response: 7161572
Conc: 62.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

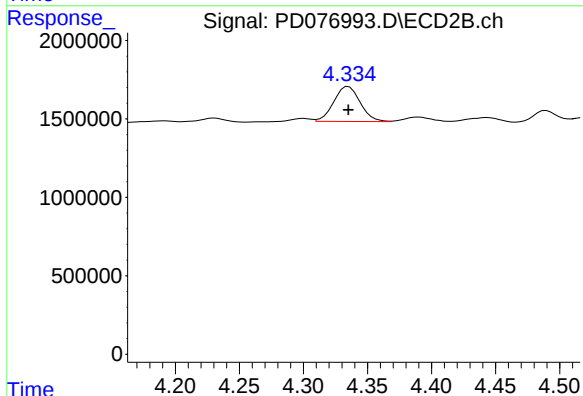


#24 Chlordane-2

R.T.: 4.335 min
Delta R.T.: 0.000 min
Response: 3199263
Conc: 58.78 ng/ml

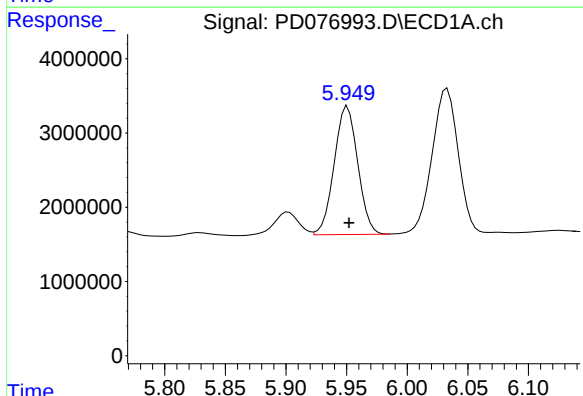


#25 Chlordane-3

R.T.: 5.951 min
Delta R.T.: -0.001 min
Response: 23368871
Conc: 49.98 ng/ml

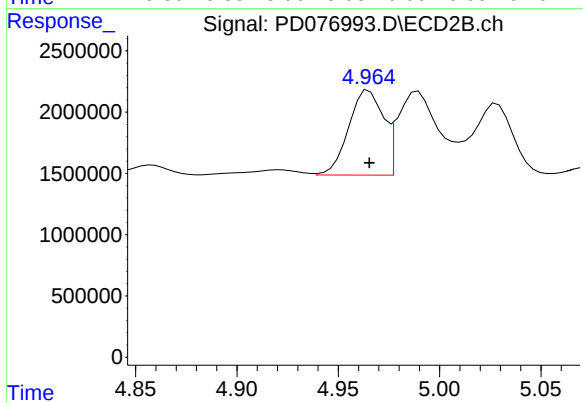

#25 Chlordane-3


R.T.: 4.965 min
Delta R.T.: 0.000 min
Response: 8241885
Conc: 51.54 ng/ml

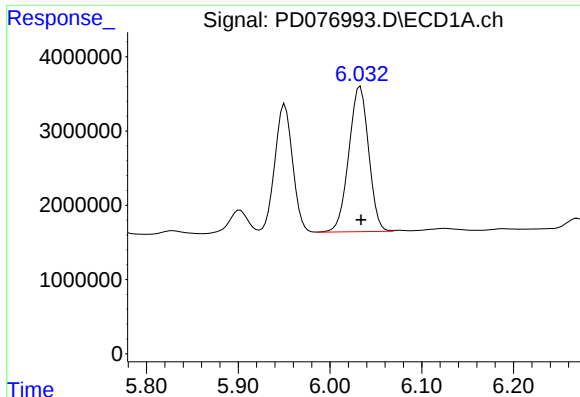

#26 Chlordane-4


R.T.: 6.033 min
Delta R.T.: 0.000 min
Response: 29317930
Conc: 51.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

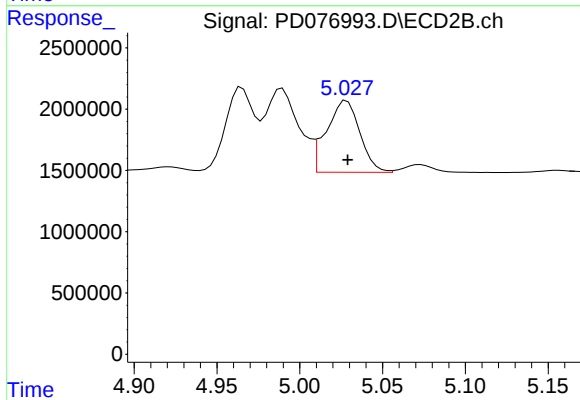


#26 Chlordane-4

R.T.: 5.028 min
Delta R.T.: 0.000 min
Response: 8221976
Conc: 51.57 ng/ml

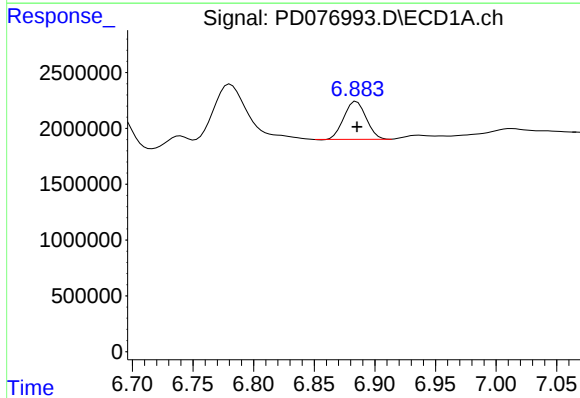


#27 Chlordane-5

R.T.: 6.885 min
Delta R.T.: 0.000 min
Response: 4351744
Conc: 46.80 ng/ml

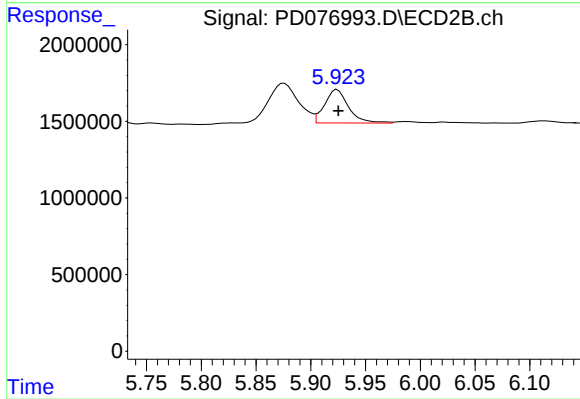

#27 Chlordane-5


R.T.: 5.924 min
Delta R.T.: 0.000 min
Response: 3309972
Conc: 57.83 ng/ml

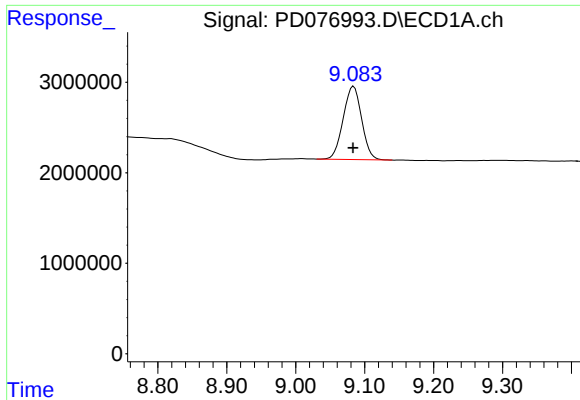

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: 0.000 min
Response: 15043183
Conc: 5.93 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

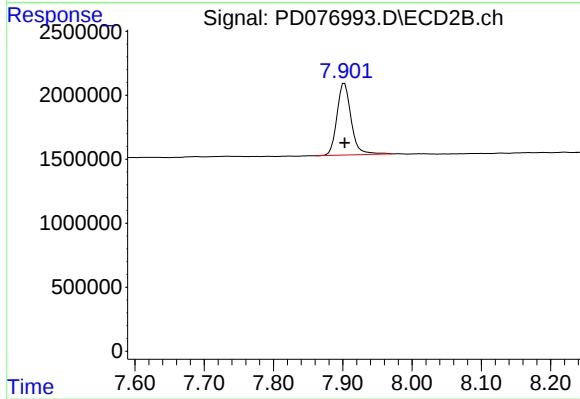

#28 Decachlorobiphenyl

R.T.: 7.902 min
Delta R.T.: 0.000 min
Response: 7980804
Conc: 6.00 ng/ml