

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080323\
 Data File : PD076991.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Aug 2023 12:52
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 03 14:01:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 13:58:43 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	2.762	111.6E6	75349463	50.000	50.000
28)	SA Decachlor...	9.083	7.903	126.8E6	66502028	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.708	3.759	52863378	24093055	500.000	500.000
24)	Chlordane-2	5.239	4.335	57661984	27211652	500.000	500.000
25)	Chlordane-3	5.952	4.965	233.8E6	79959406	500.000	500.000
26)	Chlordane-4	6.034	5.029	283.9E6	79709456	500.000	500.000
27)	Chlordane-5	6.886	5.925	46497099	28617221	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080323\
Data File : PD076991.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Aug 2023 12:52
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 03 14:01:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 13:58:43 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

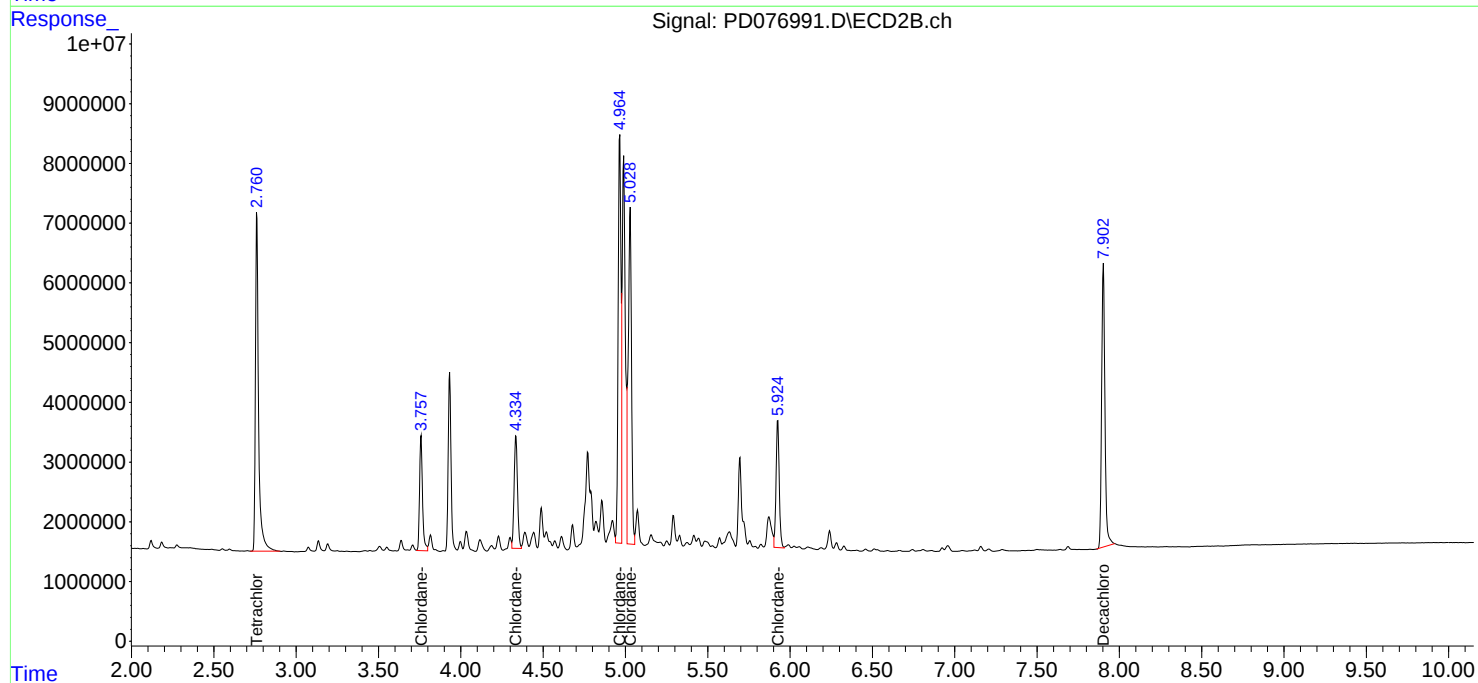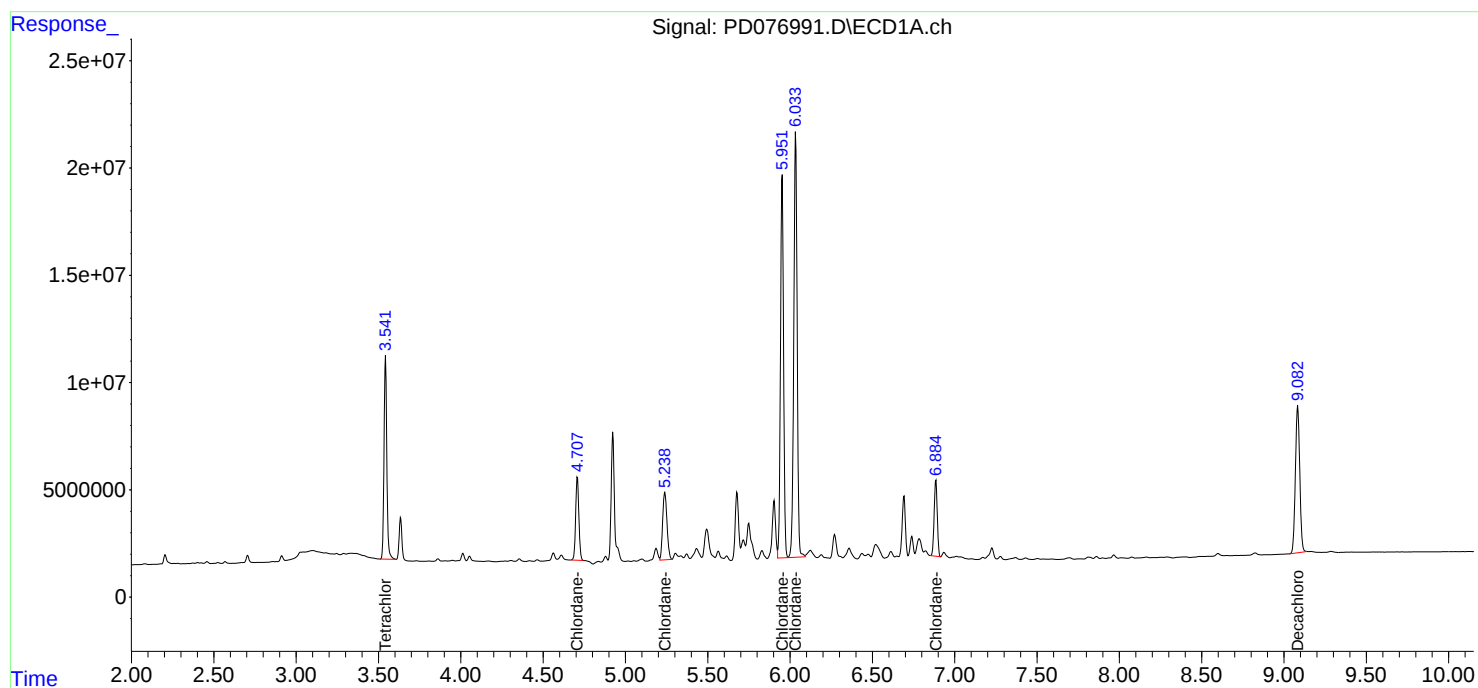


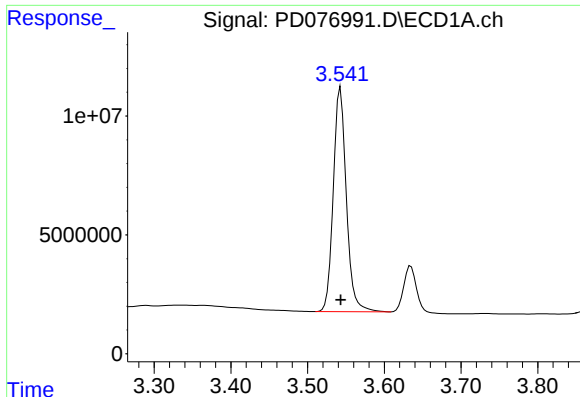

#1 Tetrachloro-m-xylene


R.T.: 3.543 min
Delta R.T.: 0.000 min
Response: 111573865
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

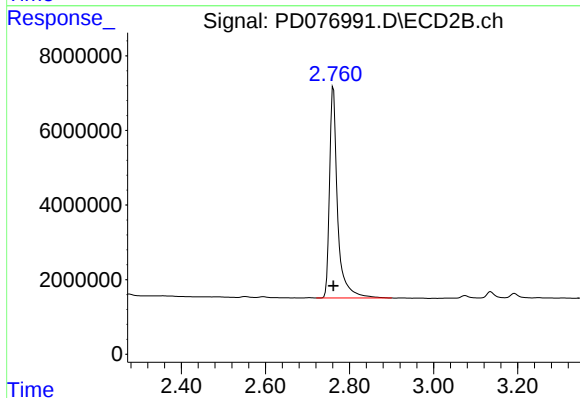


#1 Tetrachloro-m-xylene

R.T.: 2.762 min
Delta R.T.: 0.000 min
Response: 75349463
Conc: 50.00 ng/ml

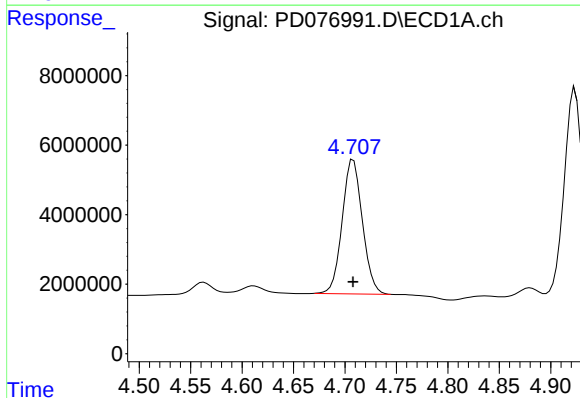


#23 Chlordane-1

R.T.: 4.708 min
Delta R.T.: 0.000 min
Response: 52863378
Conc: 500.00 ng/ml

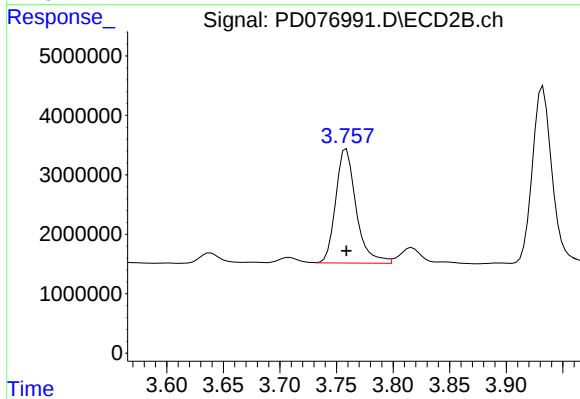

#23 Chlordane-1


R.T.: 3.759 min
Delta R.T.: 0.000 min
Response: 24093055
Conc: 500.00 ng/ml

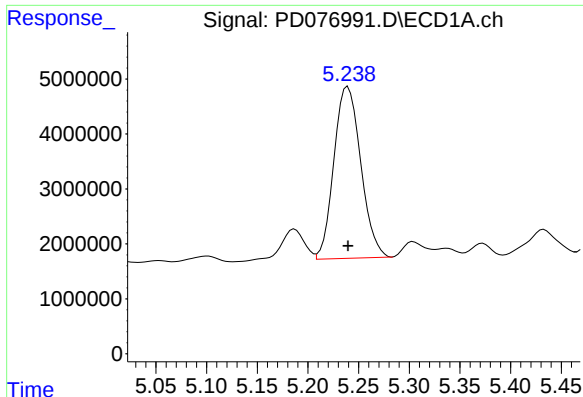

#24 Chlordane-2


R.T.: 5.239 min
Delta R.T.: 0.000 min
Response: 57661984
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

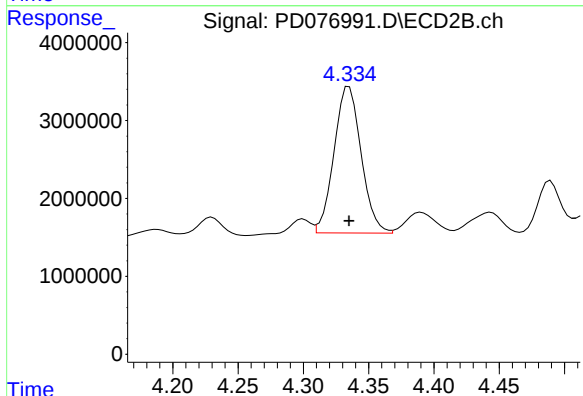


#24 Chlordane-2

R.T.: 4.335 min
Delta R.T.: 0.000 min
Response: 27211652
Conc: 500.00 ng/ml

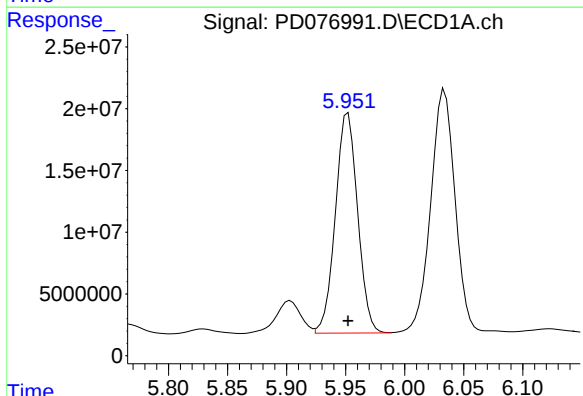


#25 Chlordane-3

R.T.: 5.952 min
Delta R.T.: 0.000 min
Response: 233782036
Conc: 500.00 ng/ml

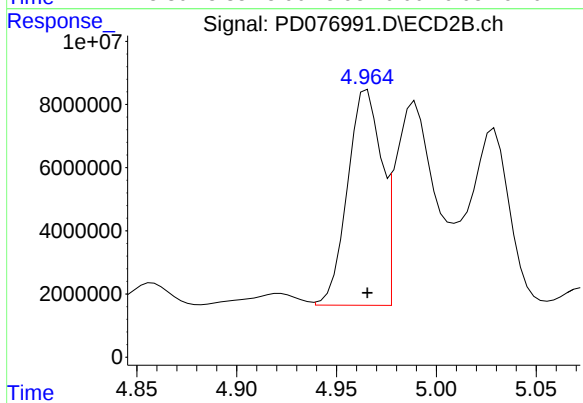

#25 Chlordane-3


R.T.: 4.965 min
Delta R.T.: 0.000 min
Response: 79959406
Conc: 500.00 ng/ml

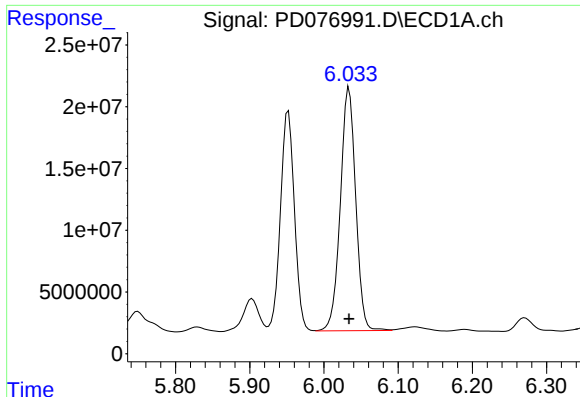

#26 Chlordane-4


R.T.: 6.034 min
Delta R.T.: 0.000 min
Response: 283853412
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

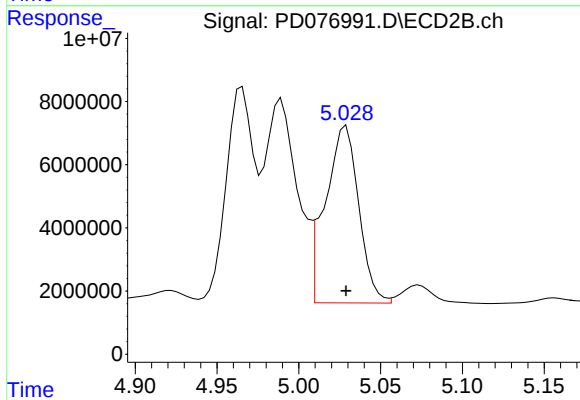


#26 Chlordane-4

R.T.: 5.029 min
Delta R.T.: 0.000 min
Response: 79709456
Conc: 500.00 ng/ml

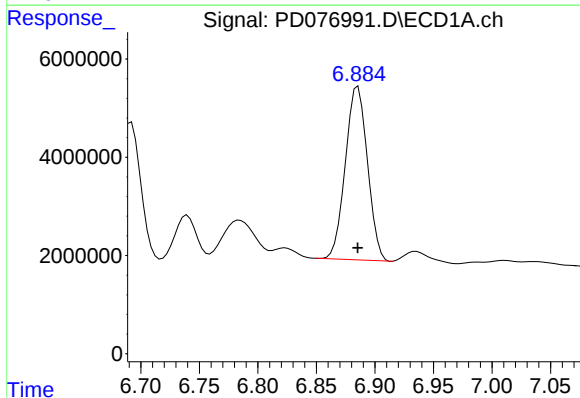


#27 Chlordane-5

R.T.: 6.886 min
Delta R.T.: 0.000 min
Response: 46497099
Conc: 500.00 ng/ml

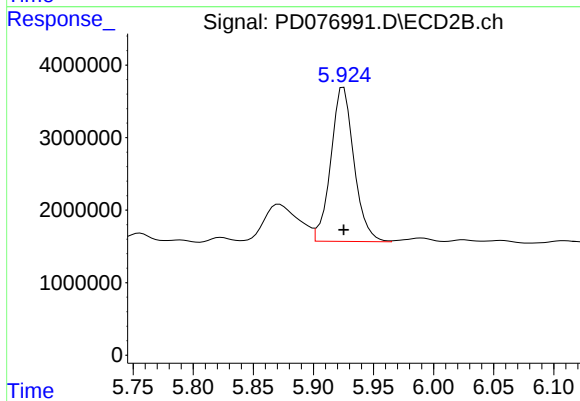

#27 Chlordane-5


R.T.: 5.925 min
Delta R.T.: 0.000 min
Response: 28617221
Conc: 500.00 ng/ml

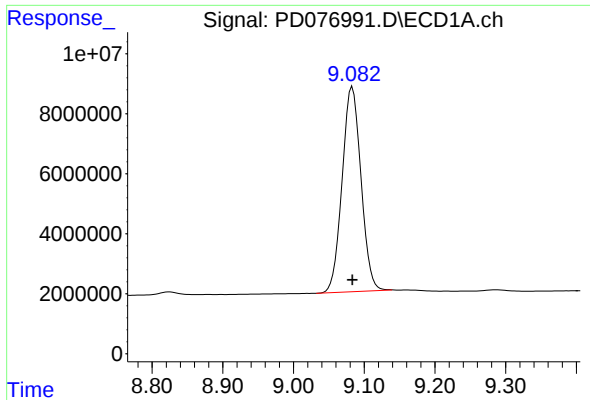

#28 Decachlorobiphenyl

R.T.: 9.083 min
Delta R.T.: 0.000 min
Response: 126790337
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

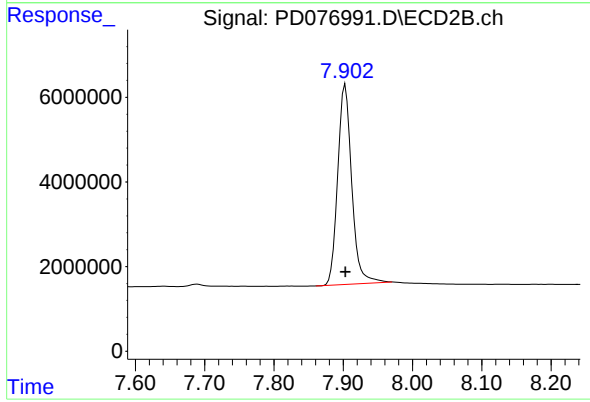

#28 Decachlorobiphenyl

R.T.: 7.903 min
Delta R.T.: 0.000 min
Response: 66502028
Conc: 50.00 ng/ml