

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080421\
 Data File : PD064712.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Aug 2021 11:00
 Operator : AR\AJ
 Sample : M3169-02MS
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C00A2MS

Manual Integrations
 APPROVED

mohammad
 8/5/2021 12:36:52 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 05 07:41:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 28 07:07:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	5.405	4.618	25057082	231.4E6	21.005	25.321
27)	SA Decachlor...	11.302	10.359	43941336	192.5E6	33.380	32.365
Target Compounds							
2)	A alpha-BHC	5.986	5.318	133.1E6	935.9E6	81.671m	75.930m
3)	MA gamma-BHC...	6.384	5.740	118.9E6	791.3E6	75.809	69.391
4)	MA Heptachlor	7.034	6.148	114.1E6	780.9E6	67.916	68.873m
5)	MB Aldrin	7.404	6.473	115.7E6	742.3E6	73.442	70.564
6)	B beta-BHC	6.643	6.114	49781005	311.0E6	63.808	51.267m
7)	B delta-BHC	6.908	6.377	119.0E6	750.5E6	68.384	69.084
8)	B Heptachlo...	7.873	7.046	105.7E6	581.9E6	61.574	62.864
9)	A Endosulfan I	8.276	7.449	93813337	491.7E6	66.550m	63.947
10)	B trans-Chl...	8.143	7.322	129.4E6	582.5E6	80.744	64.221
11)	B cis-Chlor...	8.225	7.391	99427698	589.7E6	63.813	66.290
12)	B 4,4'-DDE	8.419	7.603	172.4E6	909.9E6	119.634	120.596
13)	MA Dieldrin	8.568	7.733	210.7E6	954.4E6	141.257	118.830
14)	MA Endrin	8.806	8.023	187.5E6	795.7E6	146.472	138.519
15)	B Endosulfa...	9.042	8.331	178.4E6	708.3E6	137.405	122.702m
16)	A 4,4'-DDD	8.960	8.185	184.9E6	705.4E6	150.595	122.483
17)	MA 4,4'-DDT	9.278	8.446	184.8E6	678.9E6	141.570	123.338
18)	B Endrin al...	9.178	8.519	157.3E6	546.0E6	138.840	110.627
19)	B Endosulfa...	9.416	8.749	184.6E6	638.9E6	133.977	118.535
20)	A Methoxychlor	9.769	9.038	491.1E6	1521.9E6	686.331	594.354
21)	B Endrin ke...	9.910	9.265	222.2E6	681.2E6	146.849m	113.571m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080421\
Data File : PD064712.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Aug 2021 11:00
Operator : AR\AJ
Sample : M3169-02MS
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 05 07:41:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 28 07:07:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

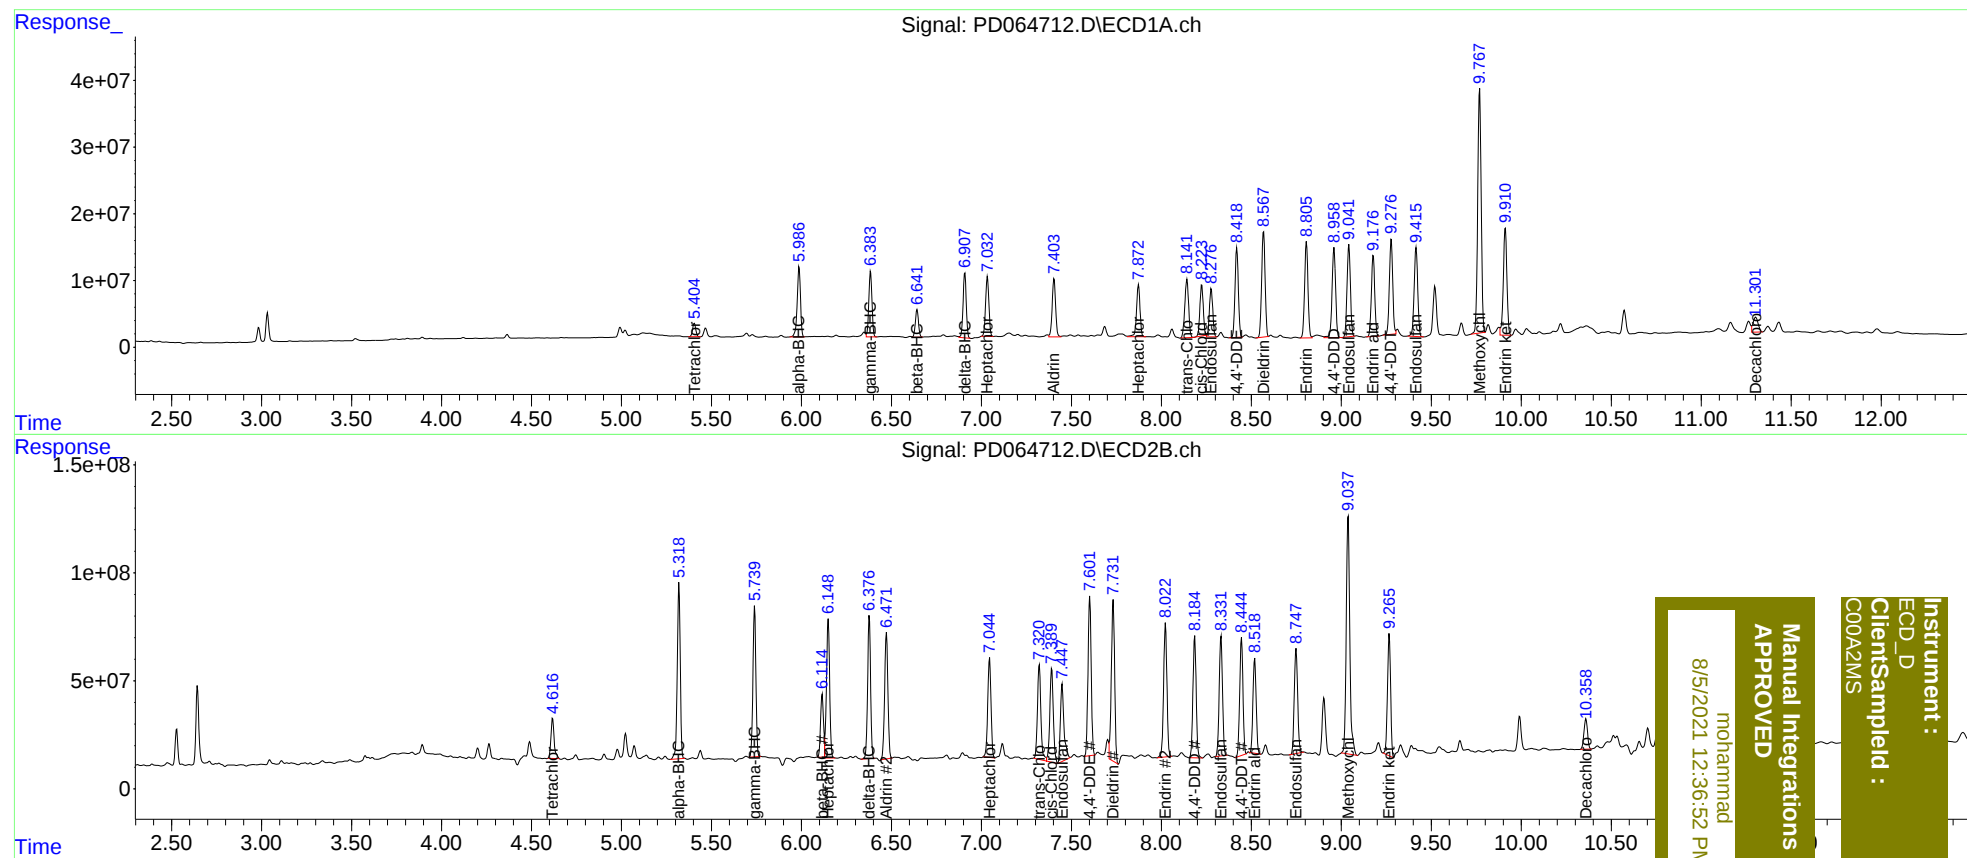

Manual Integrations
APPROVED

8/5/2021 12:36:52 PM
mohammad

Instrument :
ECD_D
ClientSampled :
C0042MS