

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080421\
 Data File : PD064711.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Aug 2021 10:44
 Operator : AR\AJ
 Sample : M3169-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C00A2

Manual Integrations
 APPROVED

mohammad
 8/5/2021 12:36:49 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 05 07:37:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 28 07:07:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	5.408	4.616	20153688	187.0E6	16.895	20.468
27)	SA Decachlor...	11.306	10.360	36143160	162.2E6	27.456	27.275
Target Compounds							
13)	MA Dieldrin	8.571	7.736	1486989	29416053	0.997	3.662m#
15)	B Endosulfa...	9.030	8.336	1802593	17522369	1.388	3.036m#
16)	A 4,4'-DDD	8.951	8.174	9414167	17984229	7.669	3.123m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080421\
Data File : PD064711.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Aug 2021 10:44
Operator : AR\AJ
Sample : M3169-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 05 07:37:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 28 07:07:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

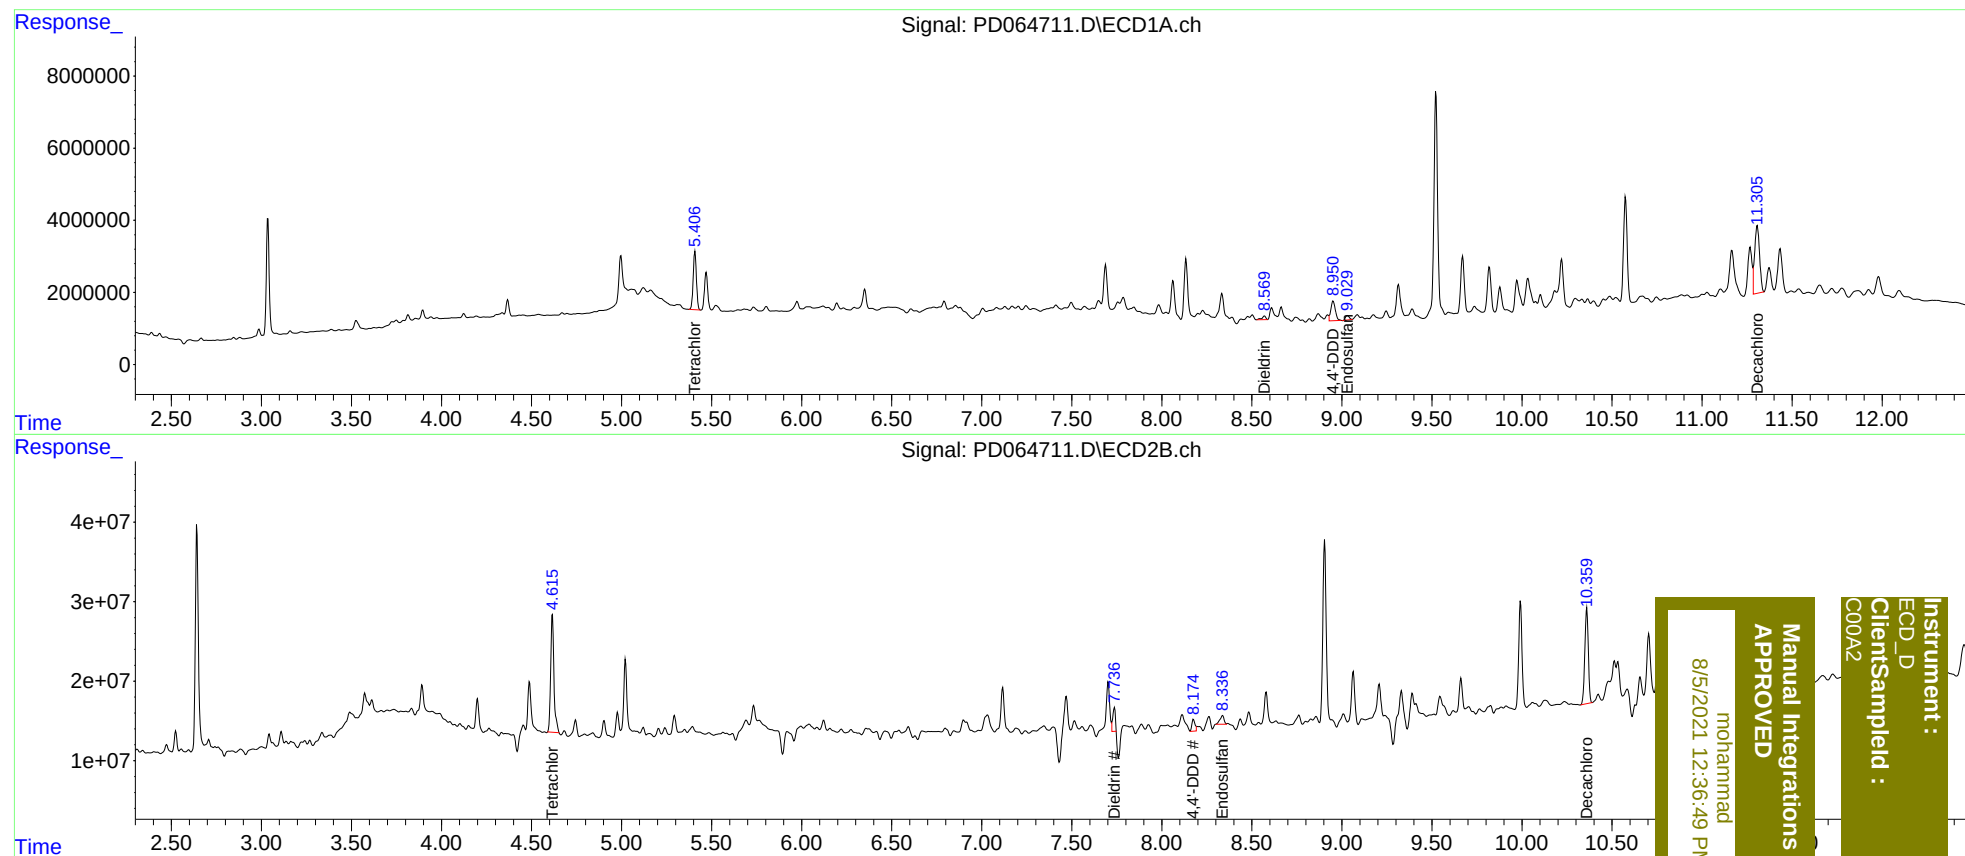

8/5/2021 12:36:49 PM

Manual Integrations
APPROVED

mohammad

Instrument :
ECD_D
ClientSampled :
C00A2