

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080422\
 Data File : PD071331.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Aug 2022 15:29
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 05 03:22:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 26 03:39:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.819	3.575	147.8E6	1300.7E6	52.109	46.205
28)	SA Decachlor...	8.020	9.106	122.4E6	482.5E6	44.149	46.608
Target Compounds							
23)	Chlordane-1	3.835	4.739	46163955	373.4E6	429.959	493.382
24)	Chlordane-2	4.417	5.272	49351394	282.3E6	421.054m	471.212
25)	Chlordane-3	5.057	5.983	159.0E6	961.7E6	465.620	518.720m
26)	Chlordane-4	5.121	6.062	147.0E6	1106.8E6	463.282	507.800
27)	Chlordane-5	6.024	6.923	55112181	228.0E6	455.820	504.100m



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080422\
Data File : PD071331.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Aug 2022 15:29
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 05 03:22:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072622.M
Quant Title : GC Extractables
QLast Update : Tue Jul 26 03:39:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

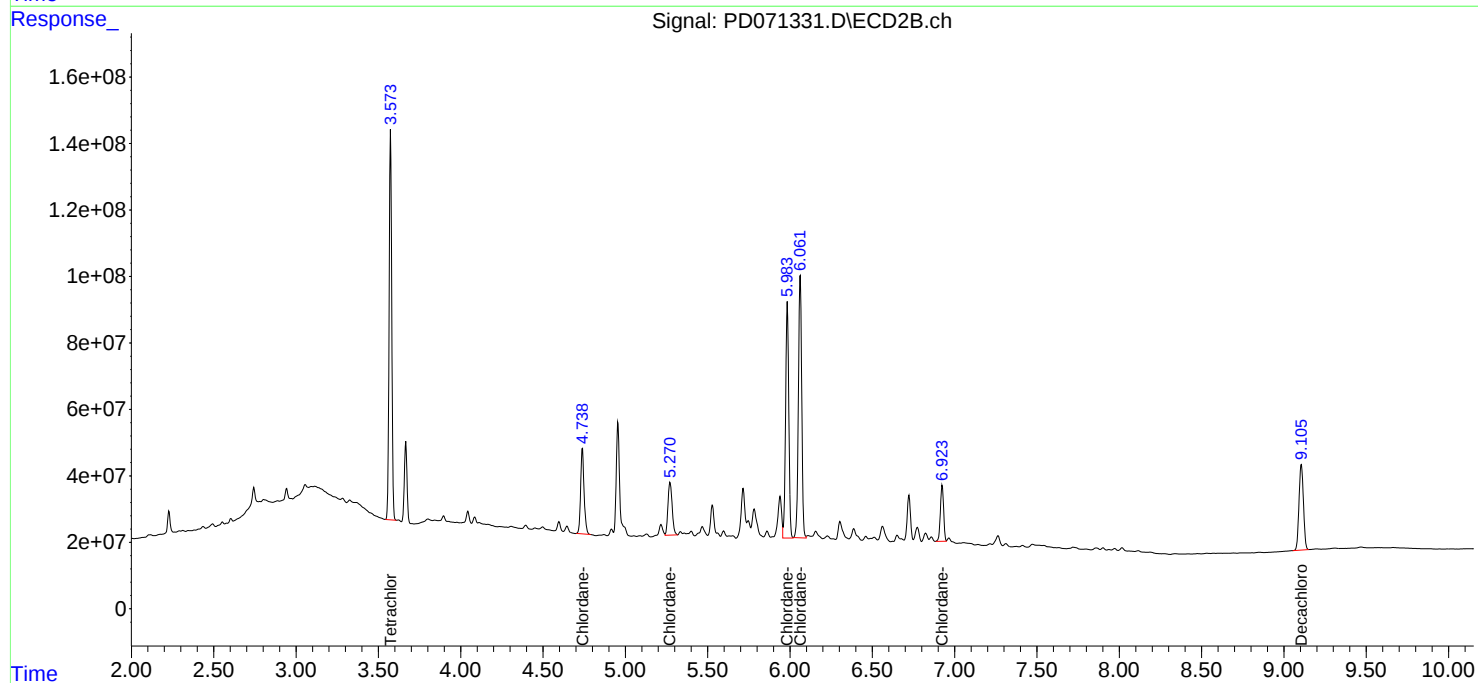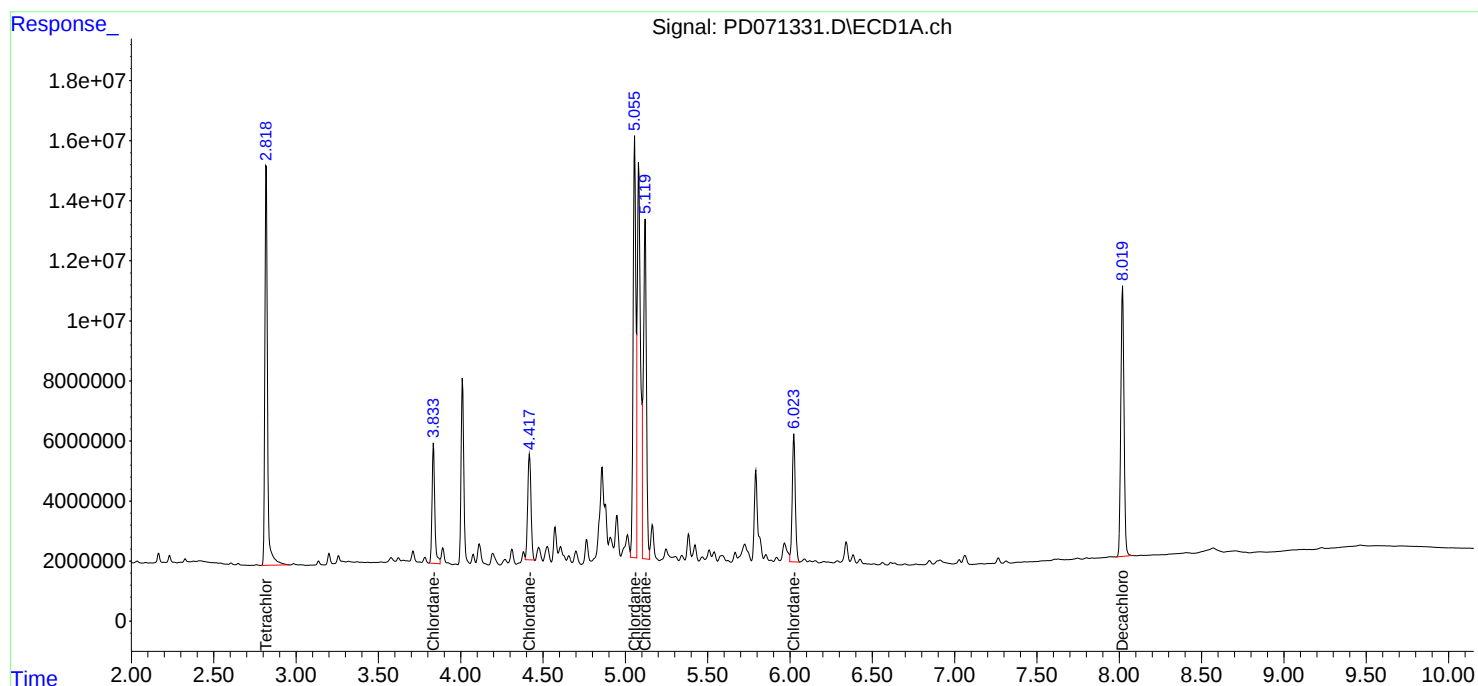


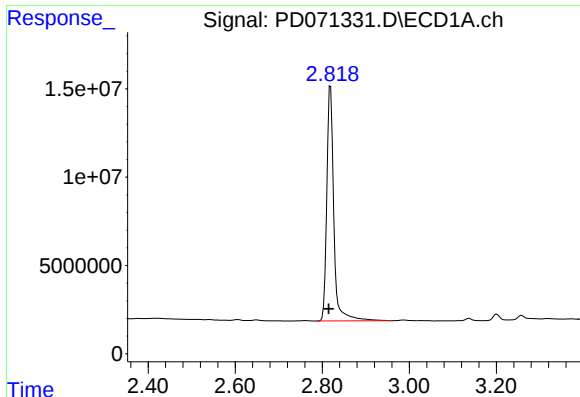

#1 Tetrachloro-m-xylene


R.T.: 2.819 min
Delta R.T.: 0.004 min
Response: 147778928
Conc: 52.11 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

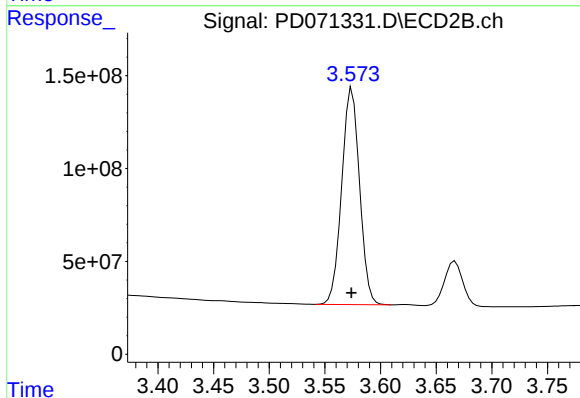


#1 Tetrachloro-m-xylene

R.T.: 3.575 min
Delta R.T.: 0.000 min
Response: 1300672621
Conc: 46.21 ng/ml

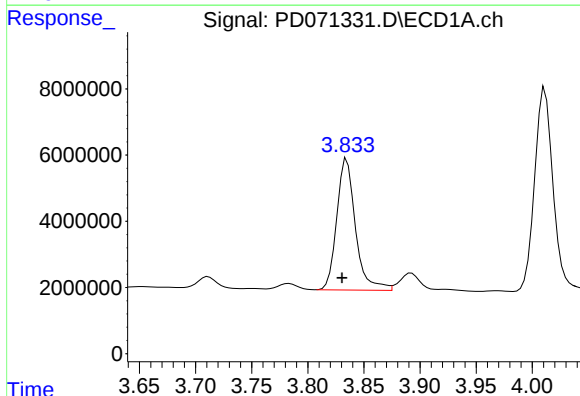


#23 Chlordane-1

R.T.: 3.835 min
Delta R.T.: 0.004 min
Response: 46163955
Conc: 429.96 ng/ml

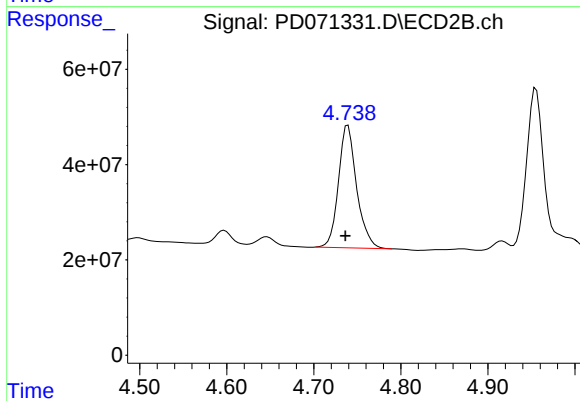

#23 Chlordane-1


R.T.: 4.739 min
Delta R.T.: 0.003 min
Response: 373355186
Conc: 493.38 ng/ml

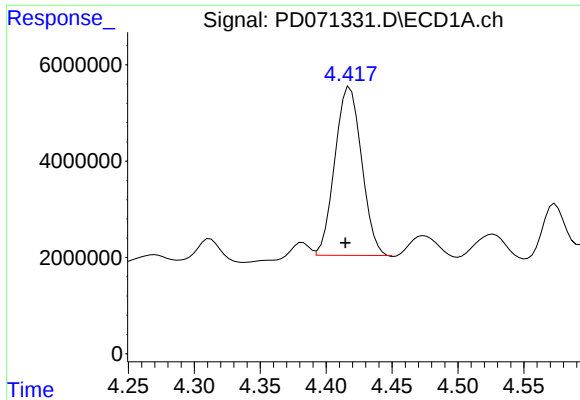

#24 Chlordane-2


R.T.: 4.417 min
Delta R.T.: 0.002 min
Response: 49351394
Conc: 421.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

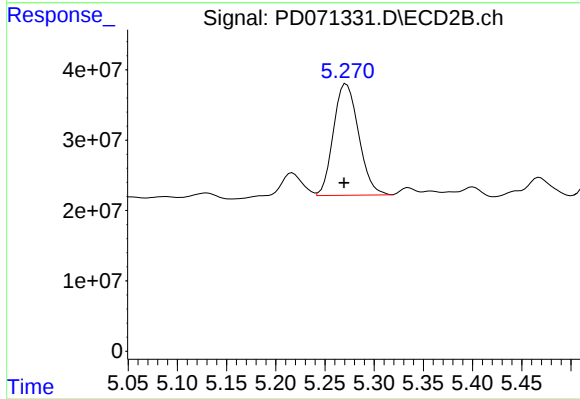


#24 Chlordane-2

R.T.: 5.272 min
Delta R.T.: 0.002 min
Response: 282259046
Conc: 471.21 ng/ml

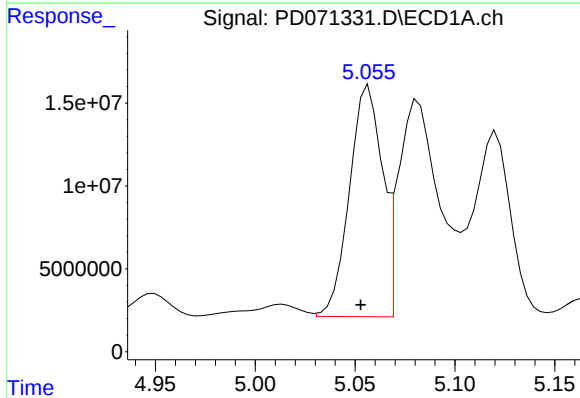


#25 Chlordane-3

R.T.: 5.057 min
Delta R.T.: 0.004 min
Response: 158989307
Conc: 465.62 ng/ml

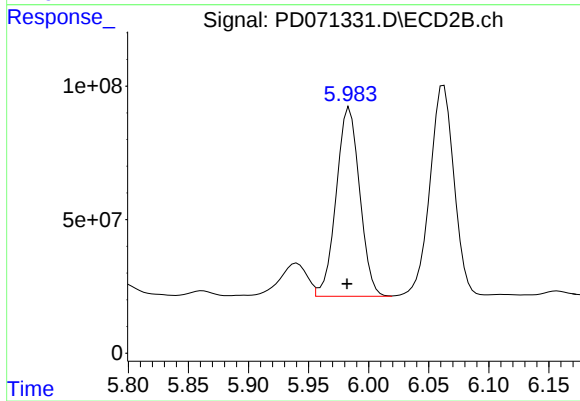

#25 Chlordane-3


R.T.: 5.983 min
Delta R.T.: 0.000 min
Response: 961668307
Conc: 518.72 ng/ml m

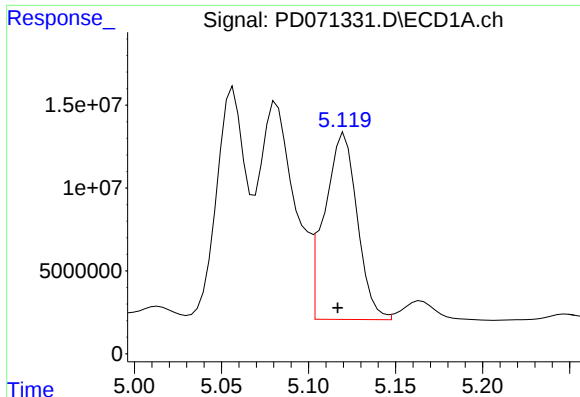

#26 Chlordane-4


R.T.: 5.121 min
Delta R.T.: 0.004 min
Response: 146978523
Conc: 463.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

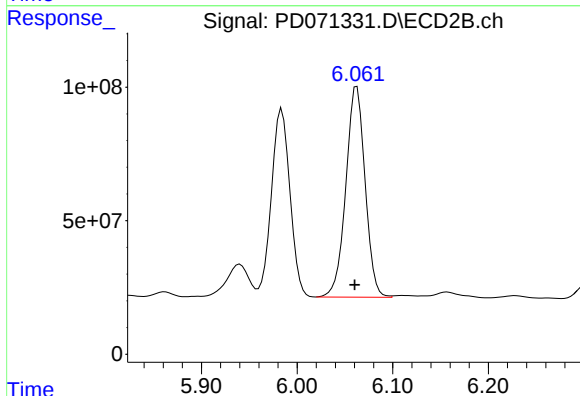


#26 Chlordane-4

R.T.: 6.062 min
Delta R.T.: 0.002 min
Response: 1106811058
Conc: 507.80 ng/ml

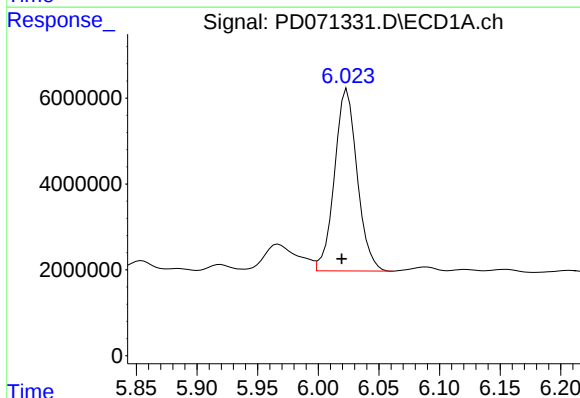


#27 Chlordane-5

R.T.: 6.024 min
Delta R.T.: 0.004 min
Response: 55112181
Conc: 455.82 ng/ml

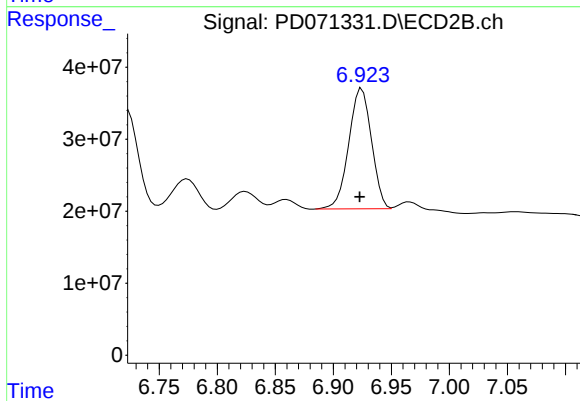

#27 Chlordane-5


R.T.: 6.923 min
Delta R.T.: 0.000 min
Response: 228002644
Conc: 504.10 ng/ml m

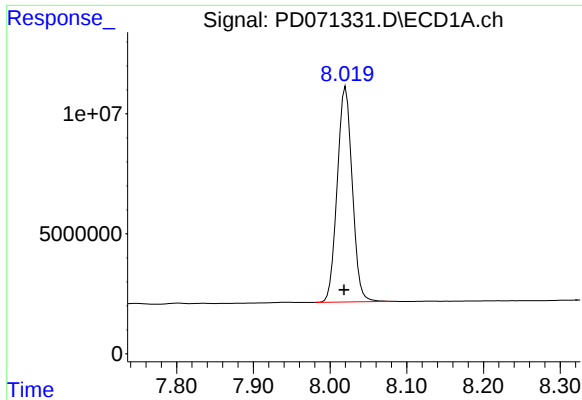

#28 Decachlorobiphenyl

R.T.: 8.020 min
Delta R.T.: 0.002 min
Response: 122448746
Conc: 44.15 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

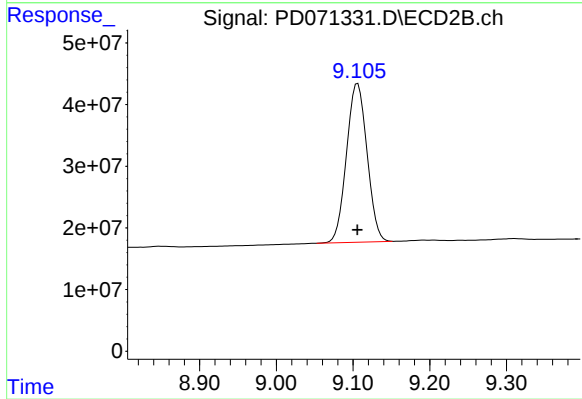

#28 Decachlorobiphenyl

R.T.: 9.106 min
Delta R.T.: 0.000 min
Response: 482514252
Conc: 46.61 ng/ml