

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080519\
 Data File : PD054195.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Aug 2019 00:45
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 04:22:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071919.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 04:33:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.313	3.982	12155651	18574155	21.120	21.322
28)	SA Decachlor...	8.007	9.025	11911955	16842523	17.695	18.168
Target Compounds							
3)	MA gamma-BHC...	4.024	0.000	448142	0	0.546	N.D. #
7)	B delta-BHC	0.000	5.013f	0	190976	N.D.	0.148 #
8)	B Heptachlo...	4.993	5.840	815375	1276600	1.075	1.056
10)	B gamma-Chl...	0.000	6.085	0	334739	N.D.	0.254 #
18)	B Endrin al...	6.285f	0.000	204257	0	0.322	N.D. #
21)	B Endrin ke...	0.000	7.723f	0	684370	N.D.	0.563 #
22)	Mirex	0.000	8.181f	0	336585	N.D.	0.365 #
25)	Chlordane-3	0.000	6.085	0	334739	N.D.	1.912 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080519\
Data File : PD054195.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Aug 2019 00:45
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 04:22:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071919.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 04:33:23 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

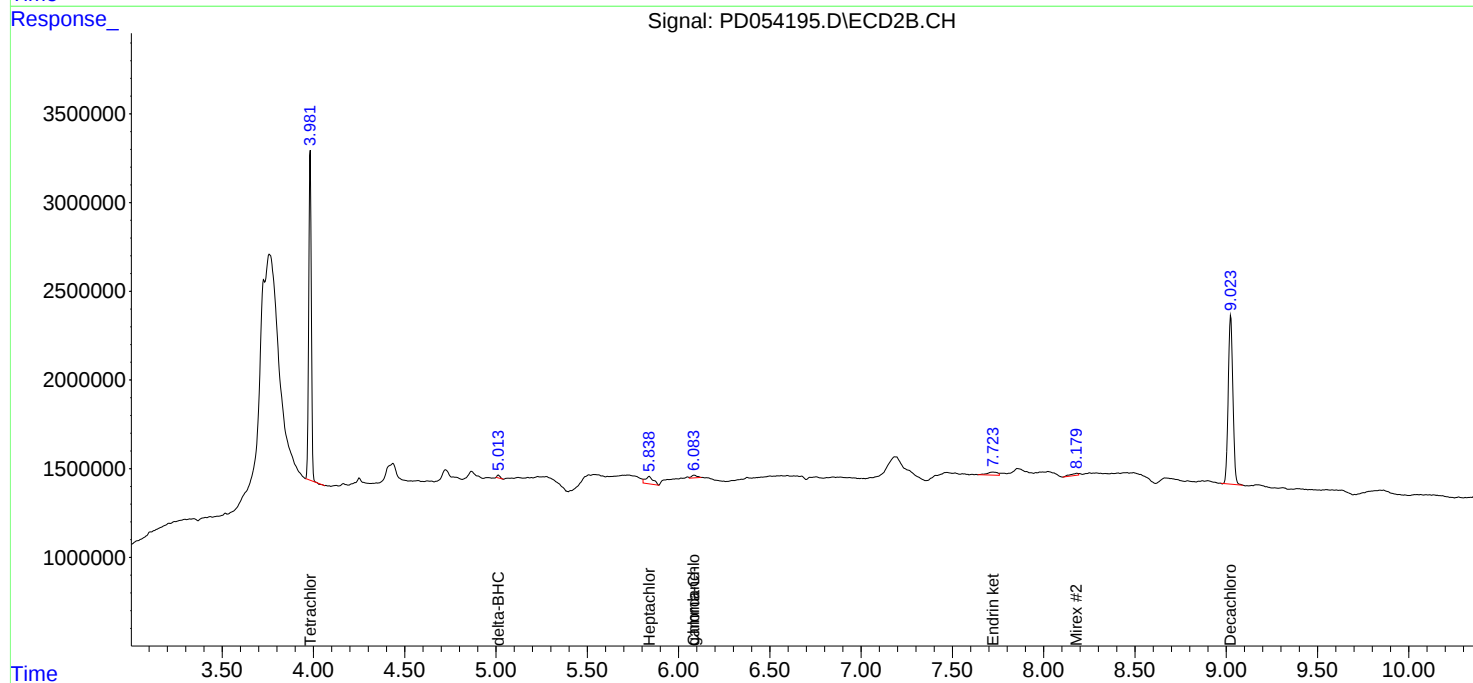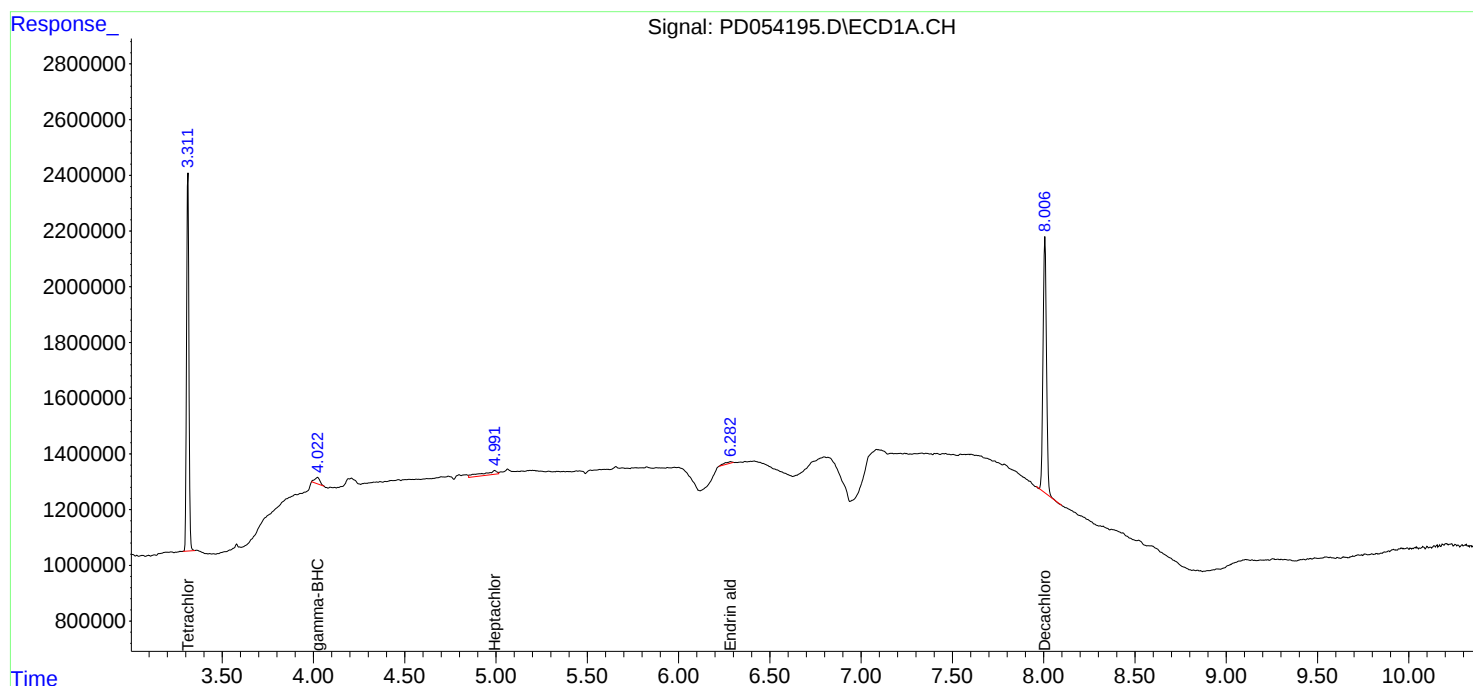


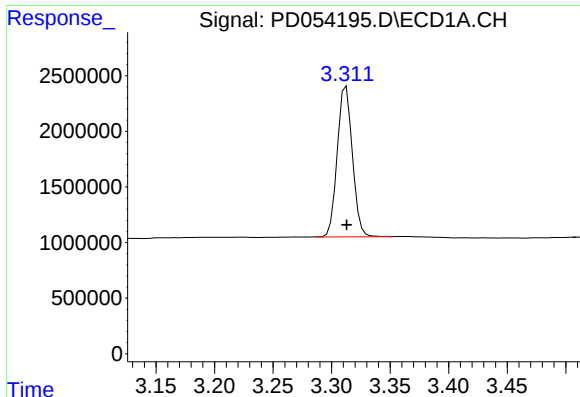

#1 Tetrachloro-m-xylene


R.T.: 3.313 min
Delta R.T.: 0.000 min
Response: 12155651
Conc: 21.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

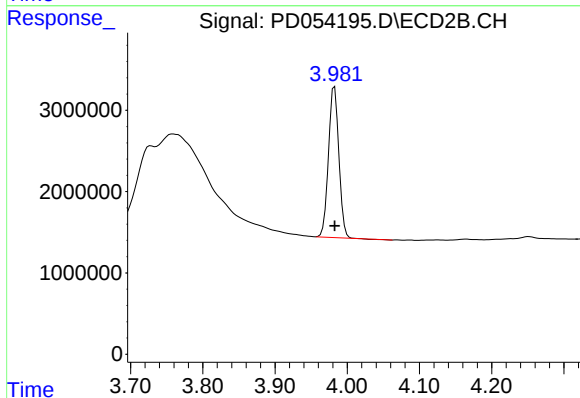


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 18574155
Conc: 21.32 ng/ml

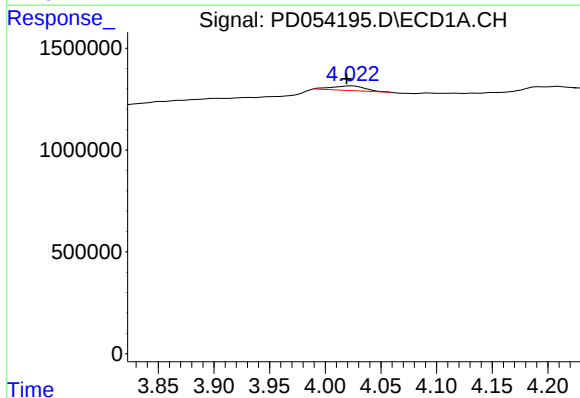


#3 gamma-BHC (Lindane)

R.T.: 4.024 min
Delta R.T.: 0.004 min
Response: 448142
Conc: 0.55 ng/ml

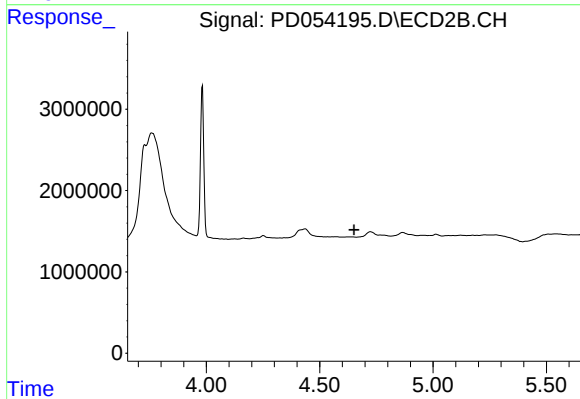

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.652 min
Response: 0
Conc: N.D.

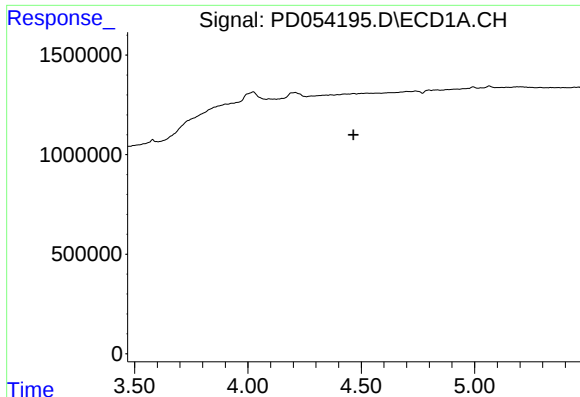

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.466 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

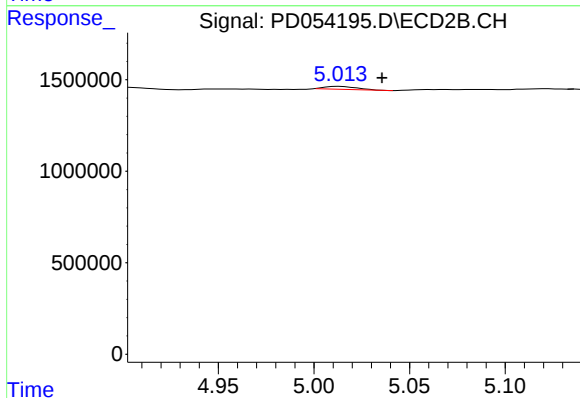


#7 delta-BHC

R.T.: 5.013 min
Delta R.T.: -0.023 min
Response: 190976
Conc: 0.15 ng/ml

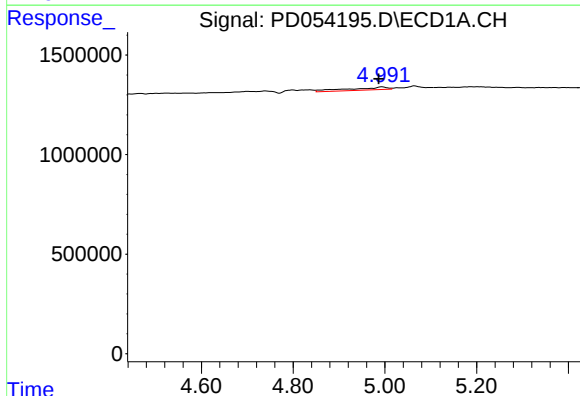


#8 Heptachlor epoxide

R.T.: 4.993 min
Delta R.T.: 0.006 min
Response: 815375
Conc: 1.07 ng/ml

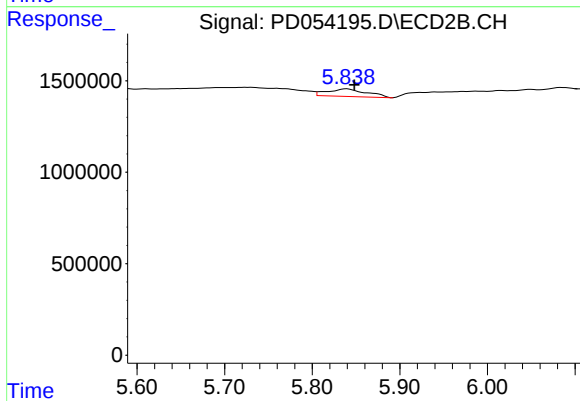

#8 Heptachlor epoxide


R.T.: 5.840 min
Delta R.T.: -0.009 min
Response: 1276600
Conc: 1.06 ng/ml

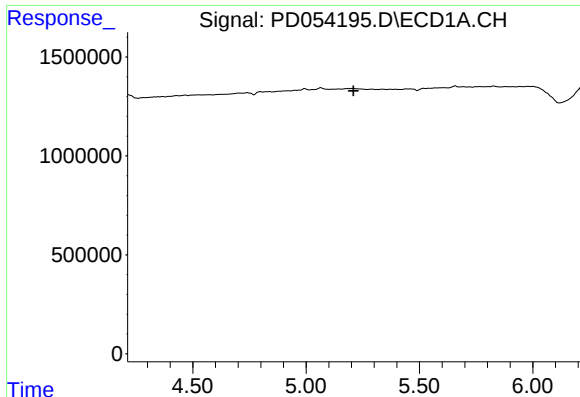

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.210 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

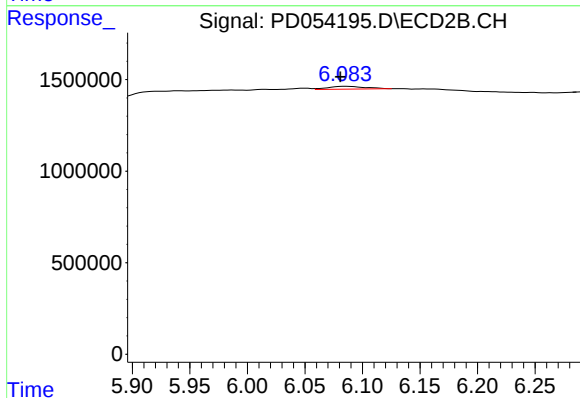


#10 gamma-Chlordane

R.T.: 6.085 min
Delta R.T.: 0.004 min
Response: 334739
Conc: 0.25 ng/ml

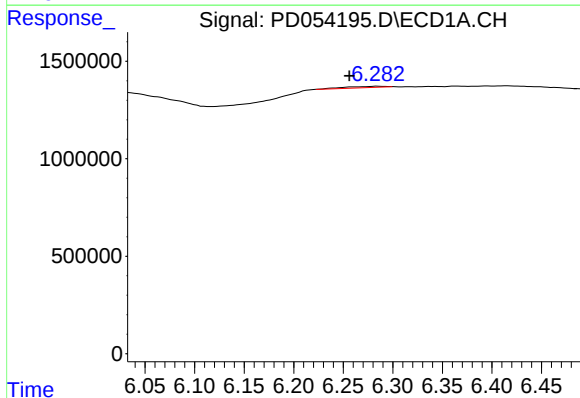


#18 Endrin aldehyde

R.T.: 6.285 min
Delta R.T.: 0.029 min
Response: 204257
Conc: 0.32 ng/ml

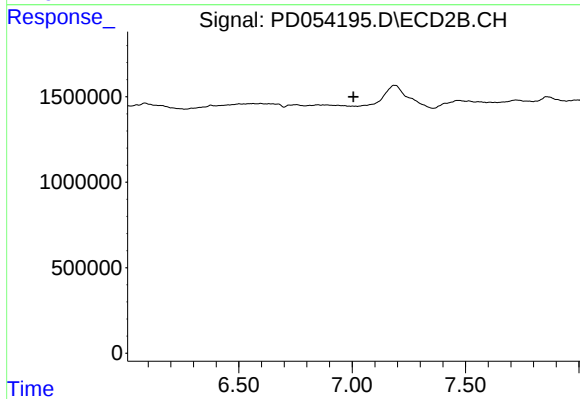

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 7.006 min
Response: 0
Conc: N.D.

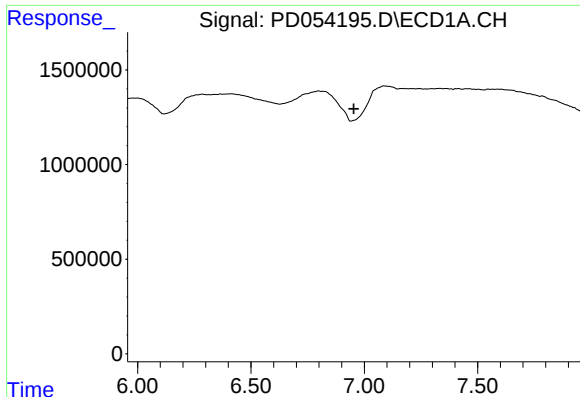

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 6.954 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

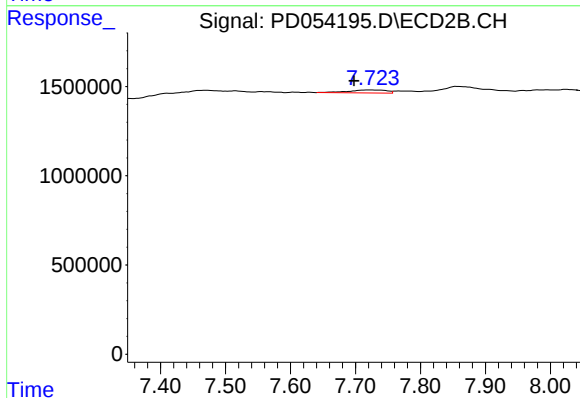


#21 Endrin ketone

R.T.: 7.723 min
Delta R.T.: 0.025 min
Response: 684370
Conc: 0.56 ng/ml

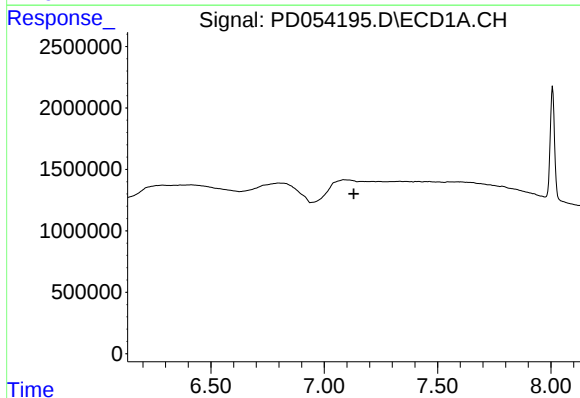


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 7.130 min
Response: 0
Conc: N.D.

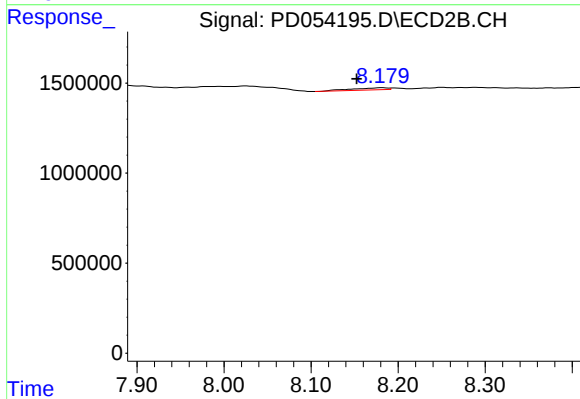

#22 Mirex


R.T.: 8.181 min
Delta R.T.: 0.029 min
Response: 336585
Conc: 0.37 ng/ml

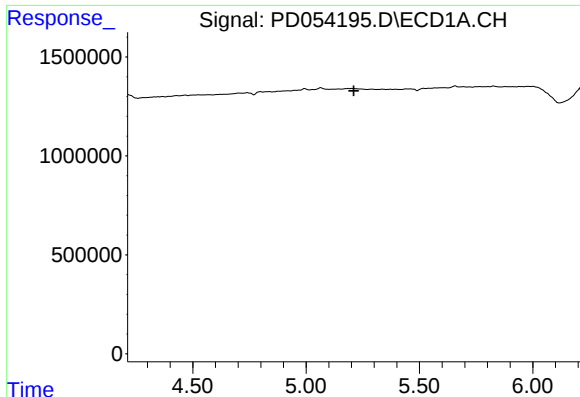

#25 Chlorine-3


R.T.: 0.000 min
Exp R.T.: 5.210 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

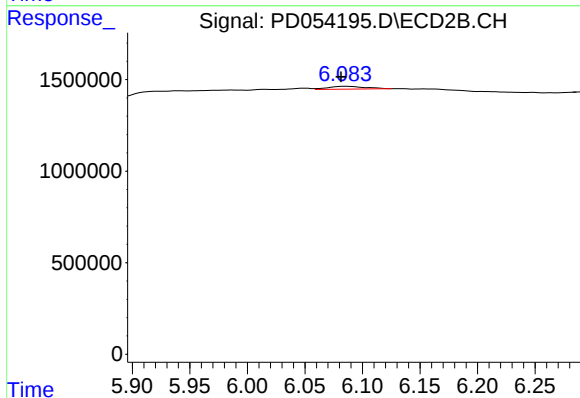


#25 Chlorine-3

R.T.: 6.085 min
Delta R.T.: 0.004 min
Response: 334739
Conc: 1.91 ng/ml

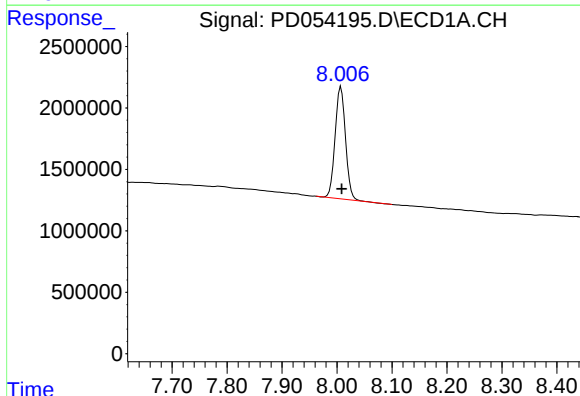

#28 Decachlorobiphenyl

R.T.: 8.007 min
Delta R.T.: -0.002 min
Response: 11911955
Conc: 17.70 ng/ml

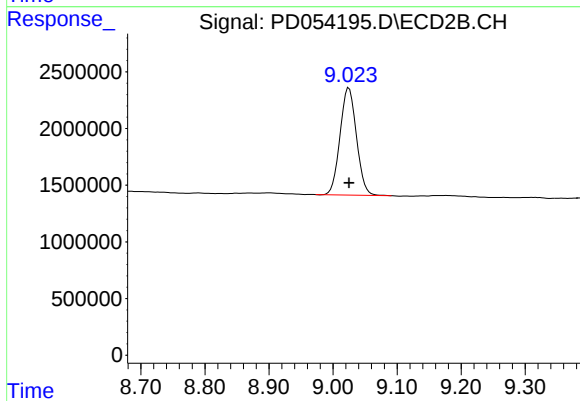

#28 Decachlorobiphenyl

R.T.: 9.025 min
Delta R.T.: 0.000 min
Response: 16842523
Conc: 18.17 ng/ml