

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080519\
 Data File : PD054188.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Aug 2019 23:08
 Operator : SM\AJ
 Sample : K4143-16
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EXT-004-SW072-073019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 04:20:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071919.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 04:33:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.312	3.983	14331153	21533104	24.900	24.719
28)	SA Decachlor...	8.007	9.024	11796123	17167650	17.523	18.518

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080519\
Data File : PD054188.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Aug 2019 23:08
Operator : SM\AJ
Sample : K4143-16
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
EXT-004-SW072-073019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 04:20:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071919.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 04:33:23 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

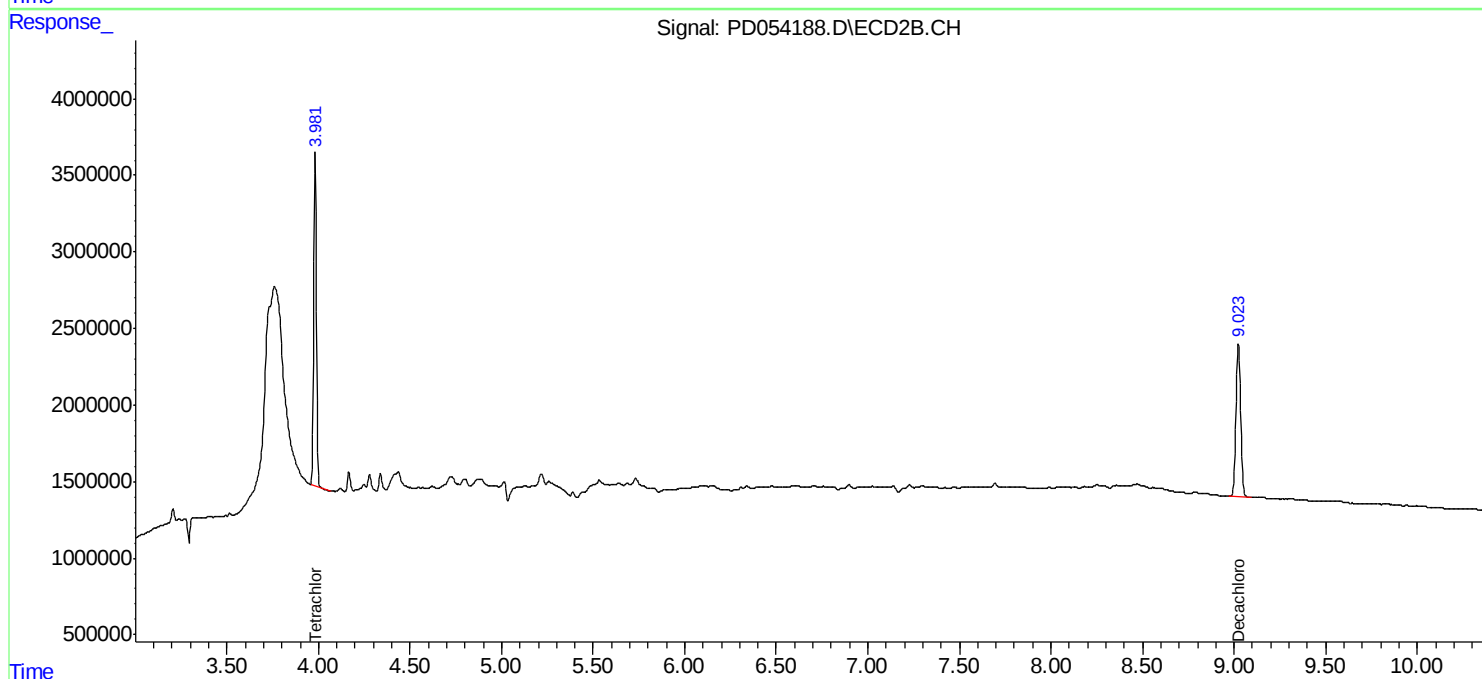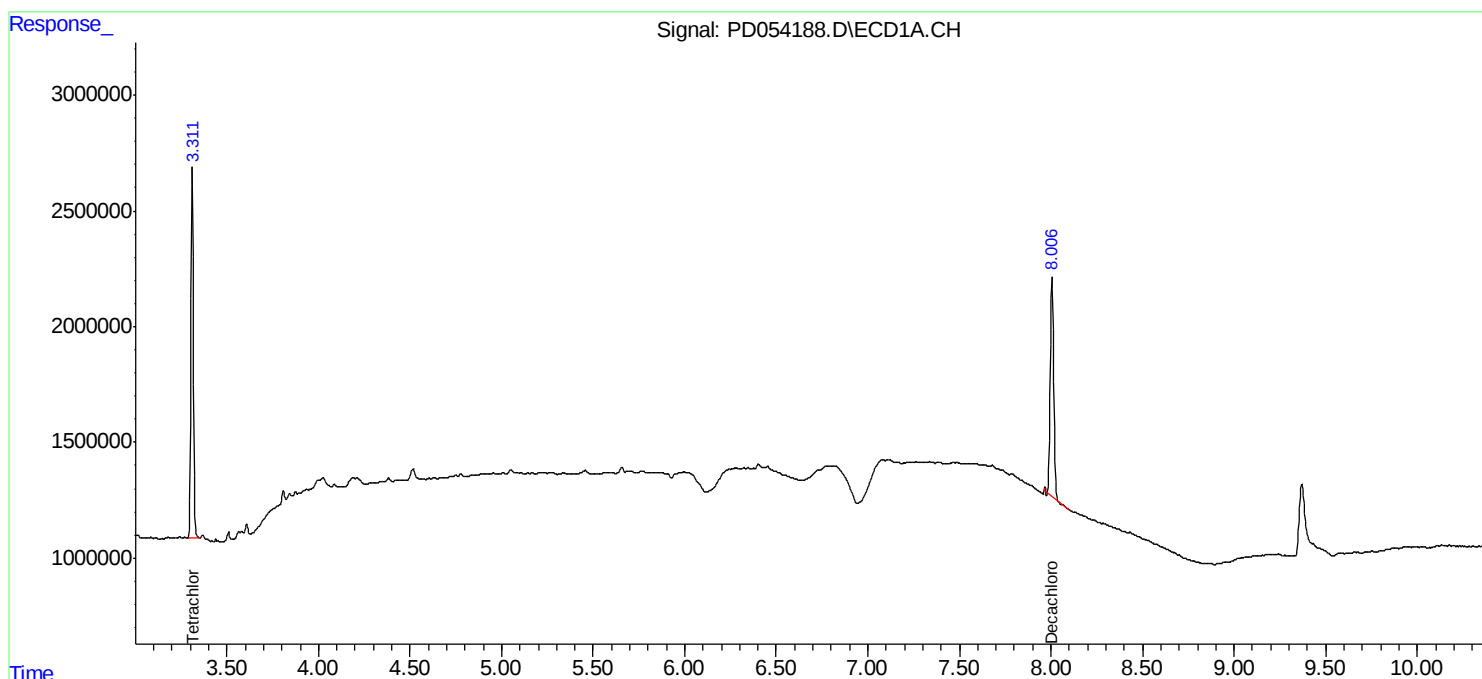


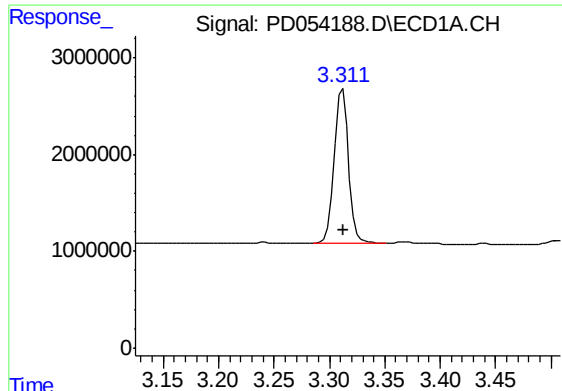

#1 Tetrachloro-m-xylene


R.T.: 3.312 min
Delta R.T.: 0.000 min
Response: 14331153
Conc: 24.90 ng/ml

Instrument :
ECD_D
ClientSampleId :
EXT-004-SW072-073019

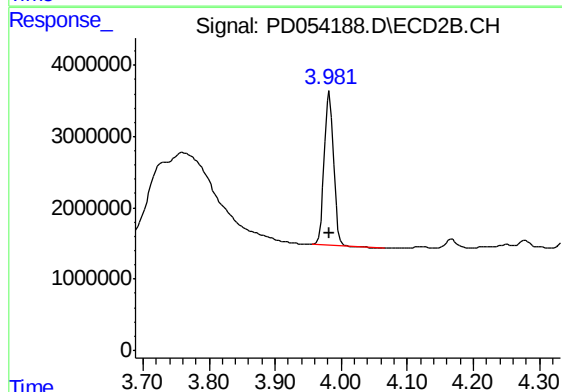


#1 Tetrachloro-m-xylene

R.T.: 3.983 min
Delta R.T.: 0.000 min
Response: 21533104
Conc: 24.72 ng/ml

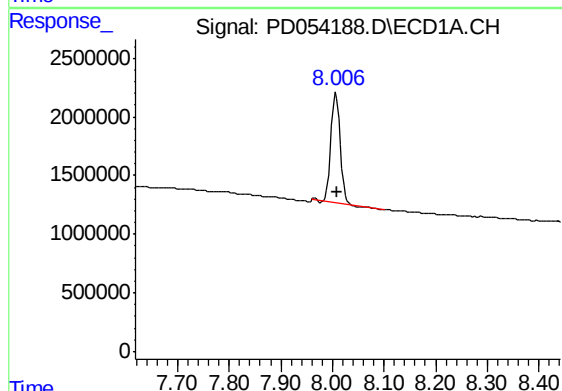

#28 Decachlorobiphenyl

R.T.: 8.007 min
Delta R.T.: -0.002 min
Response: 11796123
Conc: 17.52 ng/ml

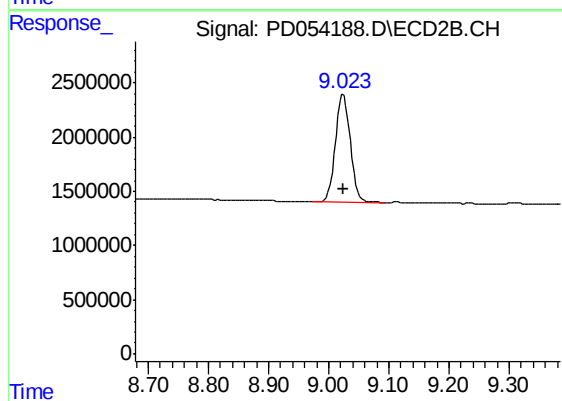

#28 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: 0.000 min
Response: 17167650
Conc: 18.52 ng/ml