

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080521\
 Data File : PD064767.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Aug 2021 13:44
 Operator : AR\AJ
 Sample : M3169-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C00A2

Manual Integrations
 APPROVED

mohammad
 8/6/2021 3:07:44 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 06:49:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 28 07:07:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	5.405	4.618	20274563	190.7E6	16.996	20.870
27)	SA Decachlor...	11.303	10.360	34409725	163.1E6	26.139m	27.427
Target Compounds							
12)	B 4,4'-DDE	8.438	7.606	2513351	18894244	1.744m	2.504 #
13)	MA Dieldrin	8.568	7.736	1145313	31771011	0.768m	3.956m#
14)	MA Endrin	8.819	8.032	923796	6816628	0.721	1.187 #
15)	B Endosulfa...	9.035	8.337	1107921	23291934	0.853m	4.035m#
16)	A 4,4'-DDD	8.948	8.175	8771696	17856008	7.146m	3.100m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080521\
Data File : PD064767.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Aug 2021 13:44
Operator : AR\AJ
Sample : M3169-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 06:49:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 28 07:07:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

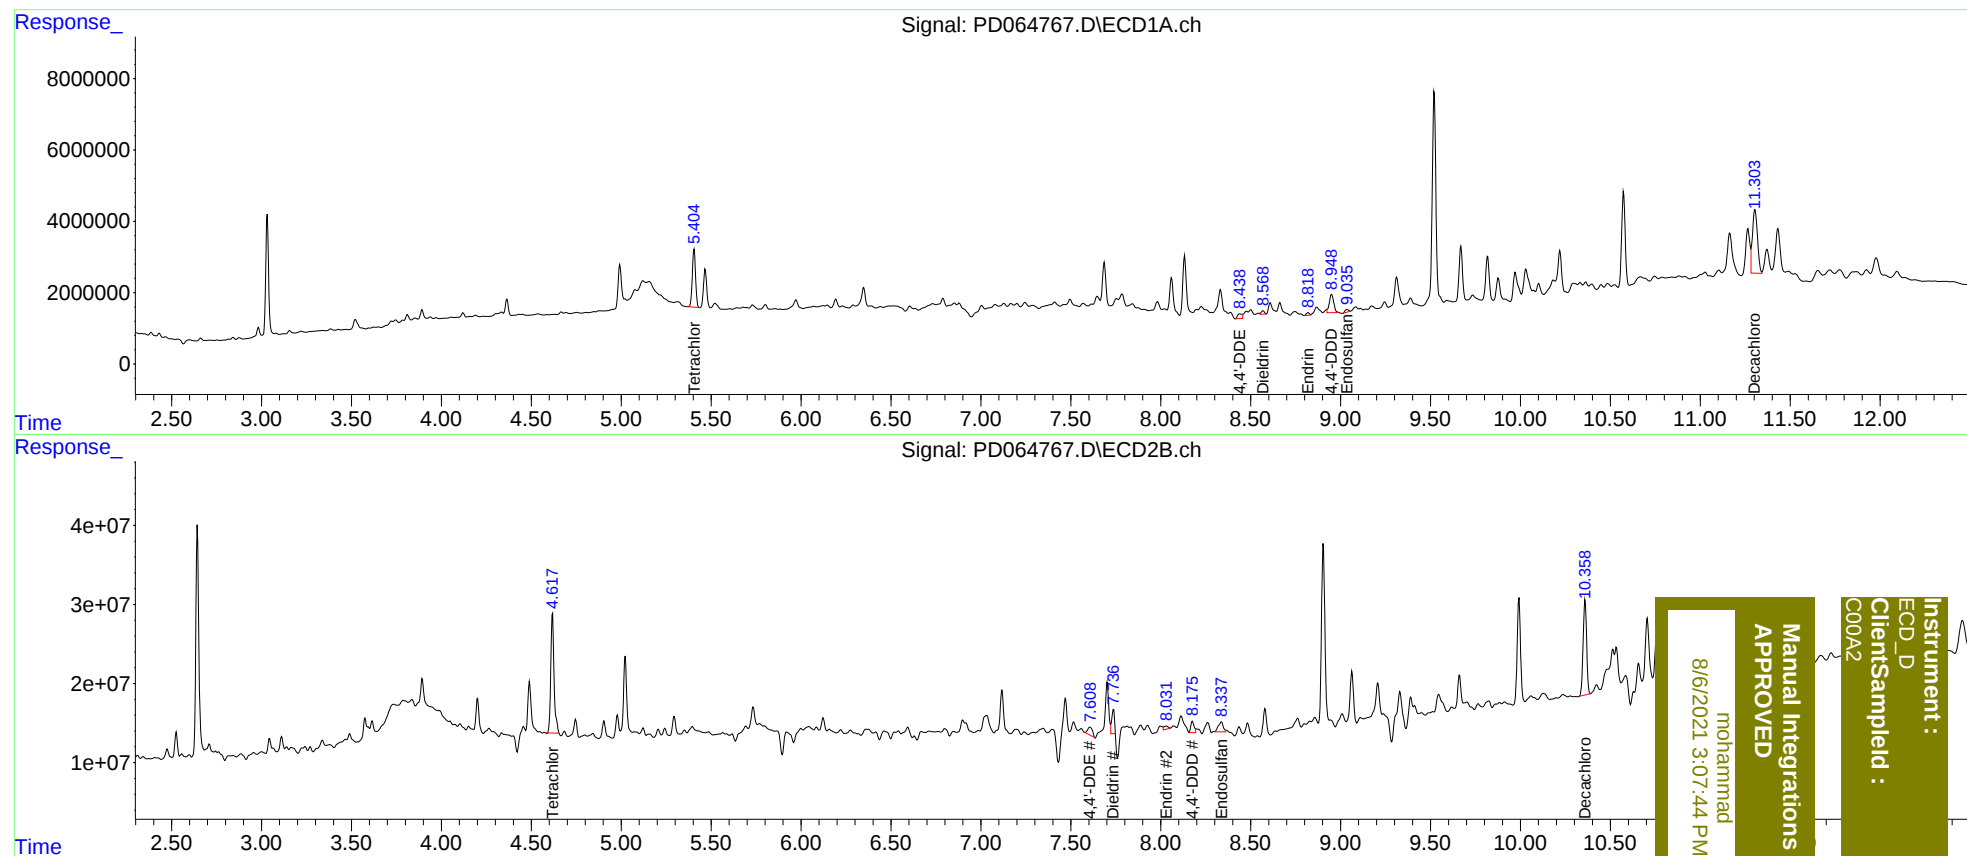

8/6/2021 3:07:44 PM

Manual Integrations
APPROVED

mohammad

Instrument :
ECD_D
ClientSampled :
C00A2