

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080522\
 Data File : PD071368.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Aug 2022 15:50
 Operator : AR\AJ
 Sample : N3980-09
 Misc : TOX MDL 50 PPB
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-WATER-03-QT3-2022

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/08/2022
 Supervised By :Ankita Jodhani 08/08/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 00:23:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX072622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 26 04:20:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	2.815	3.573	45538118	513.3E6	17.309	19.336
7) SA Decachlor...	8.013	9.101	49632927	205.5E6	19.324	21.774
Target Compounds						
2) Toxaphene-1	5.401	5.846	1038240	1848498	54.335	46.946
3) Toxaphene-2	5.637	6.490	1657146	6673696	44.171	52.108
4) Toxaphene-3	6.046	7.191	2525596	11326411	43.400	48.896m
5) Toxaphene-4	6.306	7.337	2611501	5296324	44.155	41.395
6) Toxaphene-5	6.815	7.627	2166036	8415523	36.188	50.406 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080522\
Data File : PD071368.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Aug 2022 15:50
Operator : AR\AJ
Sample : N3980-09
Misc : TOX MDL 50 PPB
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 00:23:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX072622.M
Quant Title : GC Extractables
QLast Update : Tue Jul 26 04:20:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

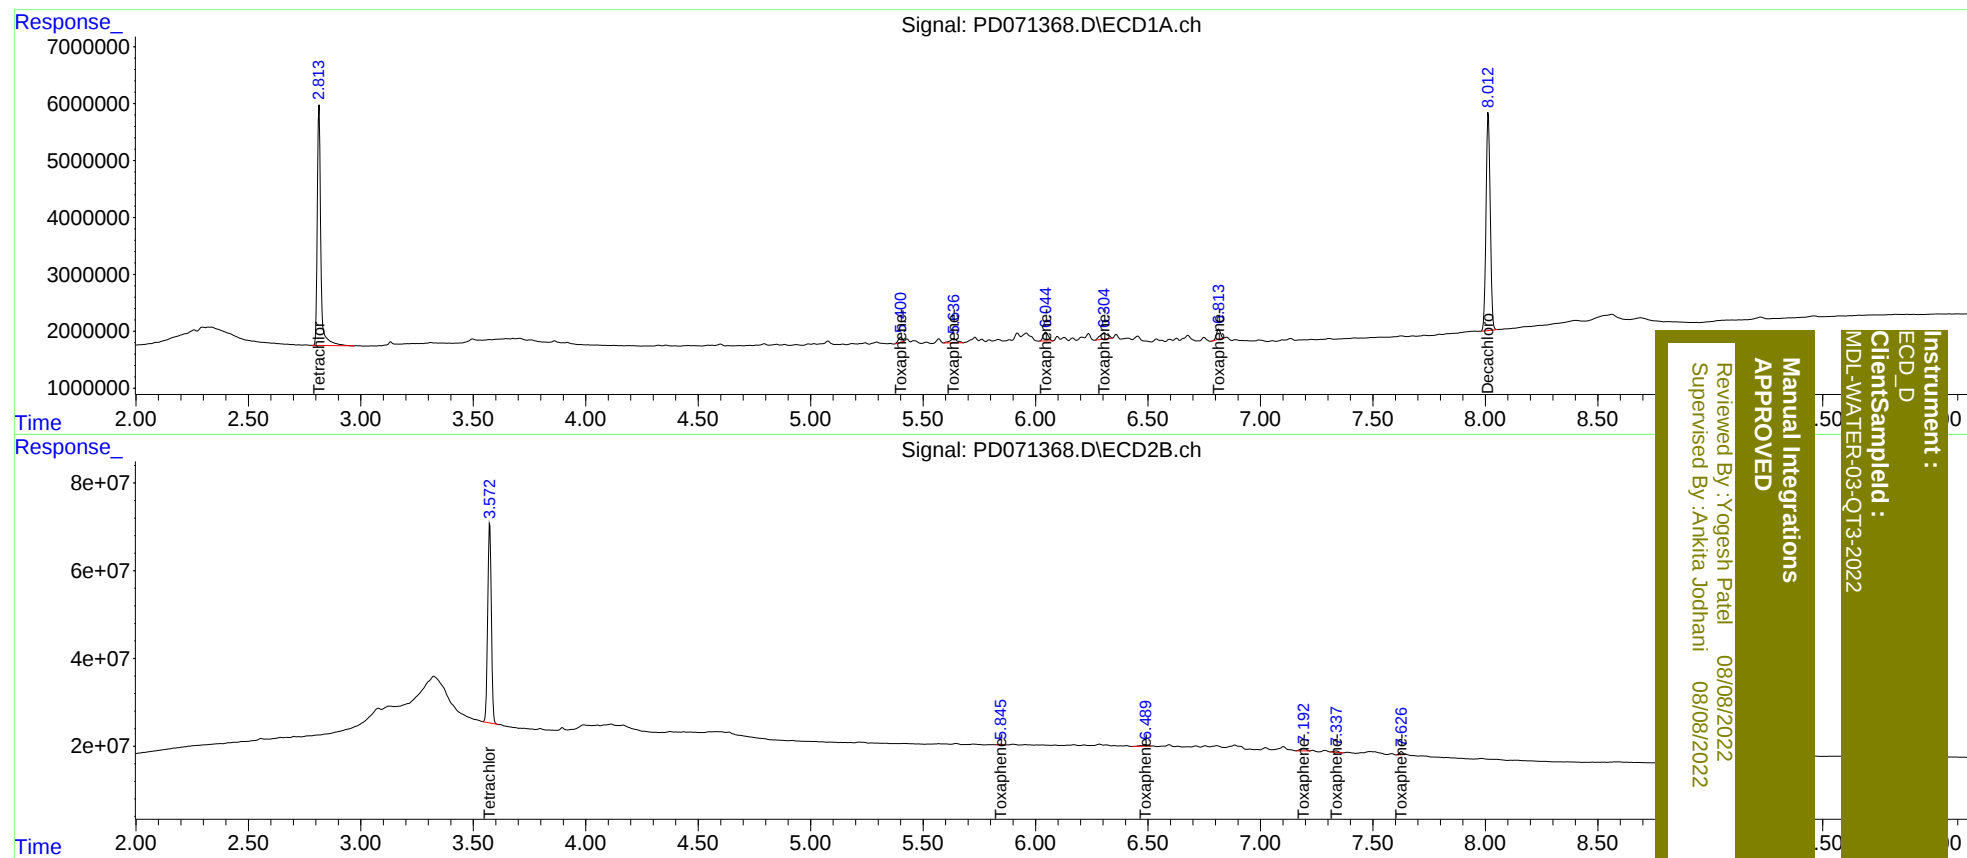

Instrument :
ECD_D
Client Sample :
MDL-WATER-03-QT3-2022

Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 08/08/2022
Supervised By : Ankita Jodhani 08/08/2022