

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080524\
 Data File : PD084212.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Aug 2024 10:46
 Operator : AR\AJ
 Sample : P3401-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E1G79

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 01:18:05 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072424CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 25 11:17:53 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.562	2.771	17994870	106.0E6	20.097	20.317
27) SA Decachlor...	9.115	7.895	19159438	62367139	9.982	10.819
Target Compounds						
7) B delta-BHC	4.791	0.000	1161810	0	0.579	N.D. #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080524\
Data File : PD084212.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Aug 2024 10:46
Operator : AR\AJ
Sample : P3401-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 01:18:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072424CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 25 11:17:53 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

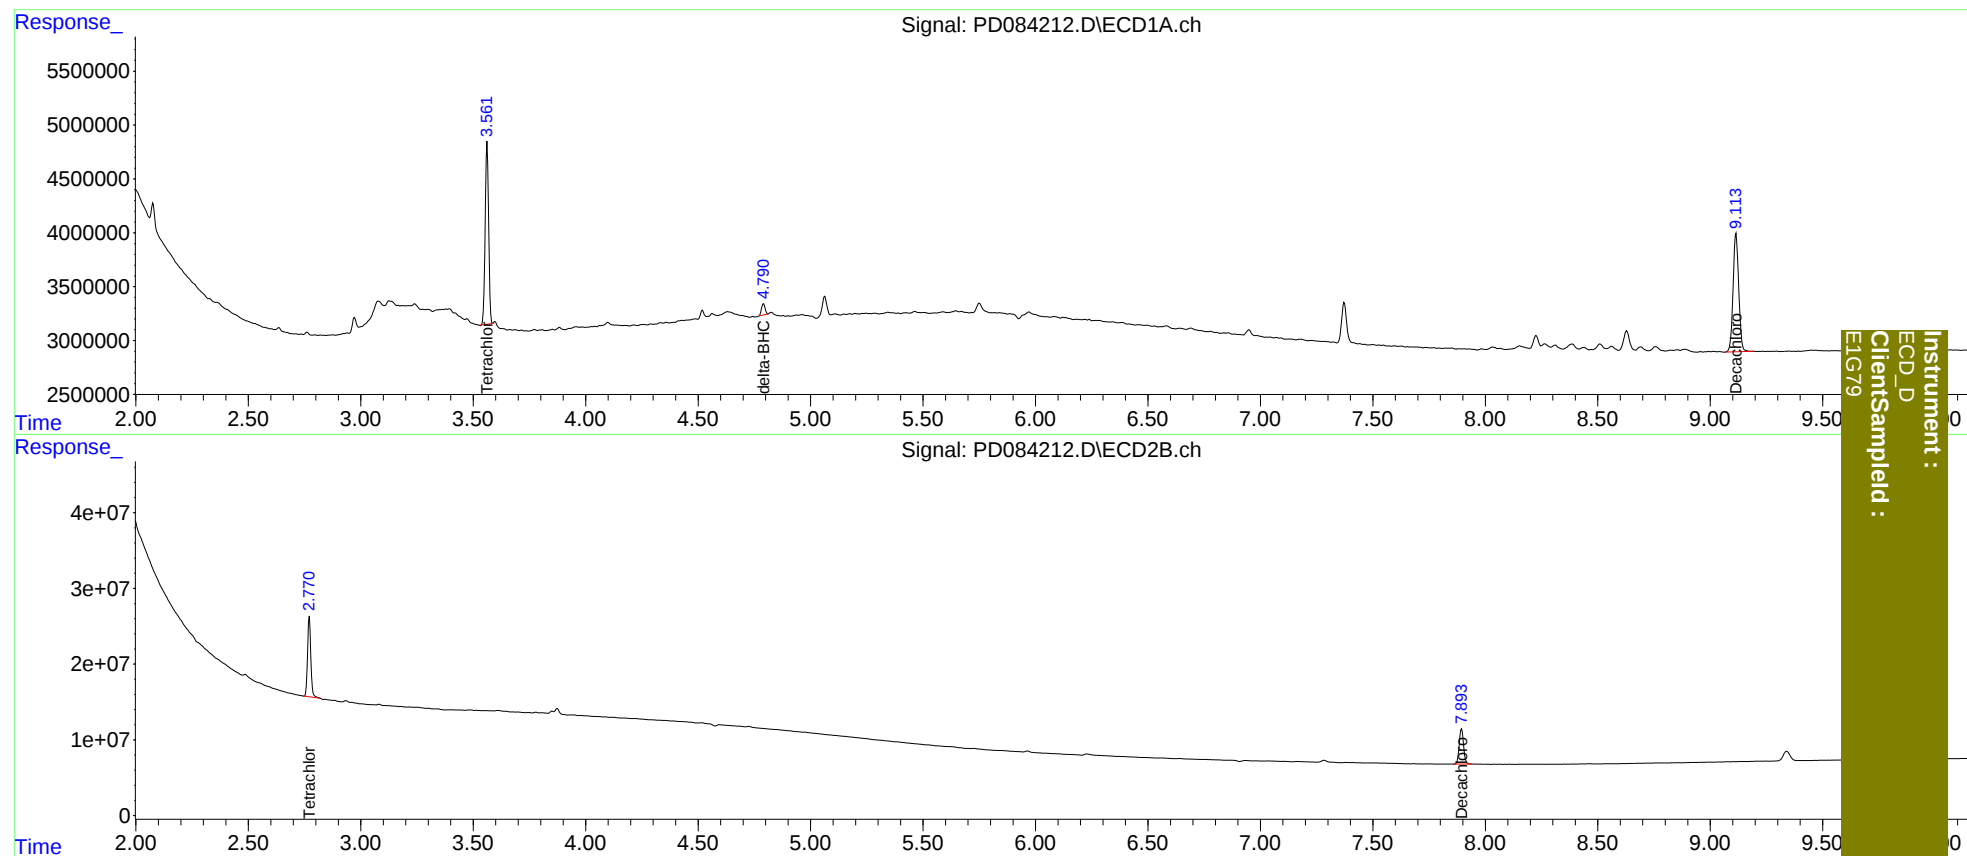


Instrument :
ECD_D
ClientSampled :
E1G79

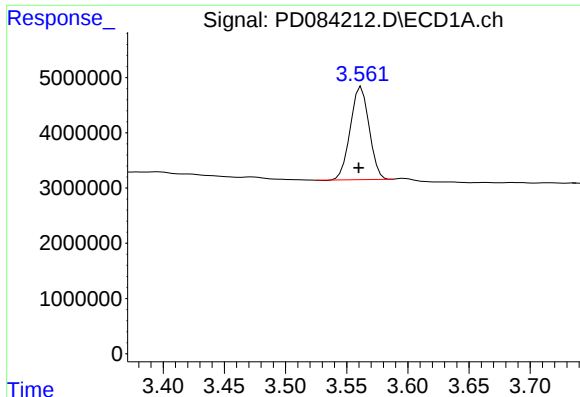

#1 Tetrachloro-m-xylene


R.T.: 3.562 min
Delta R.T.: 0.002 min
Response: 17994870
Conc: 20.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
E1G79

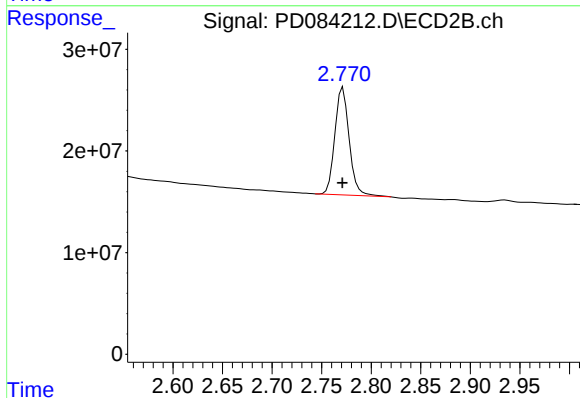


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: 0.000 min
Response: 105980679
Conc: 20.32 ng/ml

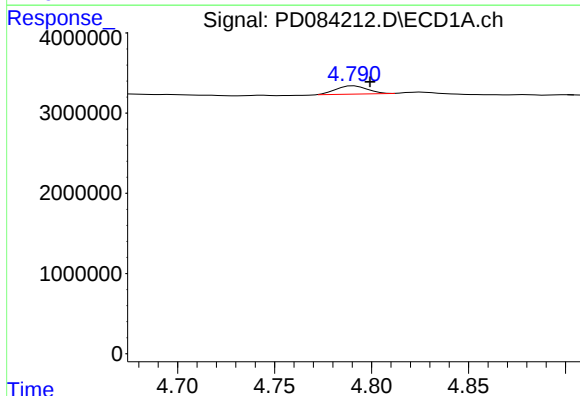


#7 delta-BHC

R.T.: 4.791 min
Delta R.T.: -0.008 min
Response: 1161810
Conc: 0.58 ng/ml

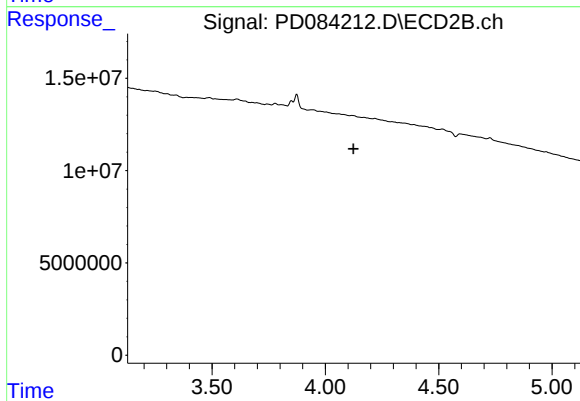

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.124 min
Response: 0
Conc: N.D.

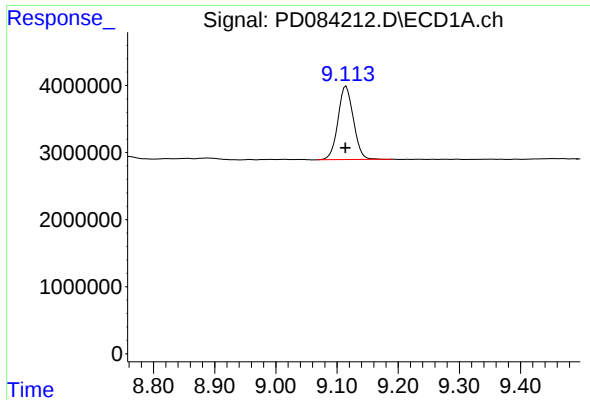

#27 Decachlorobiphenyl

R.T.: 9.115 min
Delta R.T.: 0.001 min
Response: 19159438
Conc: 9.98 ng/ml

Instrument :
ECD_D
ClientSampleId :
E1G79

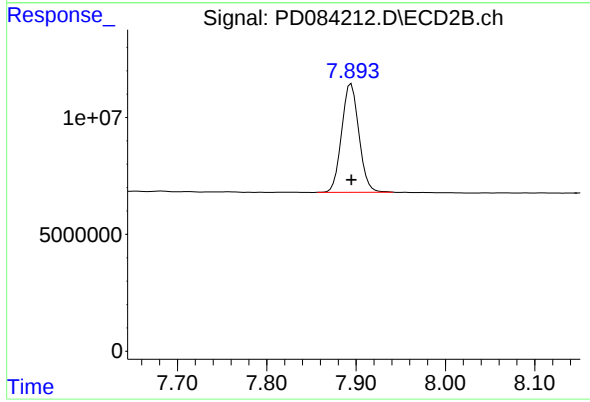

#27 Decachlorobiphenyl

R.T.: 7.895 min
Delta R.T.: 0.000 min
Response: 62367139
Conc: 10.82 ng/ml