

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080524\
 Data File : PD084213.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Aug 2024 10:59
 Operator : AR\AJ
 Sample : P3401-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E1GG3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 01:18:15 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072424CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 25 11:17:53 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.562	2.771	17276096	114.4E6	19.295	21.938
2)	SA Decachlor...	9.114	7.894	18184010	57248487	9.474	9.931
Target Compounds							
7)	B delta-BHC	4.790	0.000	1381214	0	0.689	N.D. #
10)	B trans-Chl...	5.973	0.000	2094927	0	1.181	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080524\
Data File : PD084213.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Aug 2024 10:59
Operator : AR\AJ
Sample : P3401-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 01:18:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072424CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 25 11:17:53 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

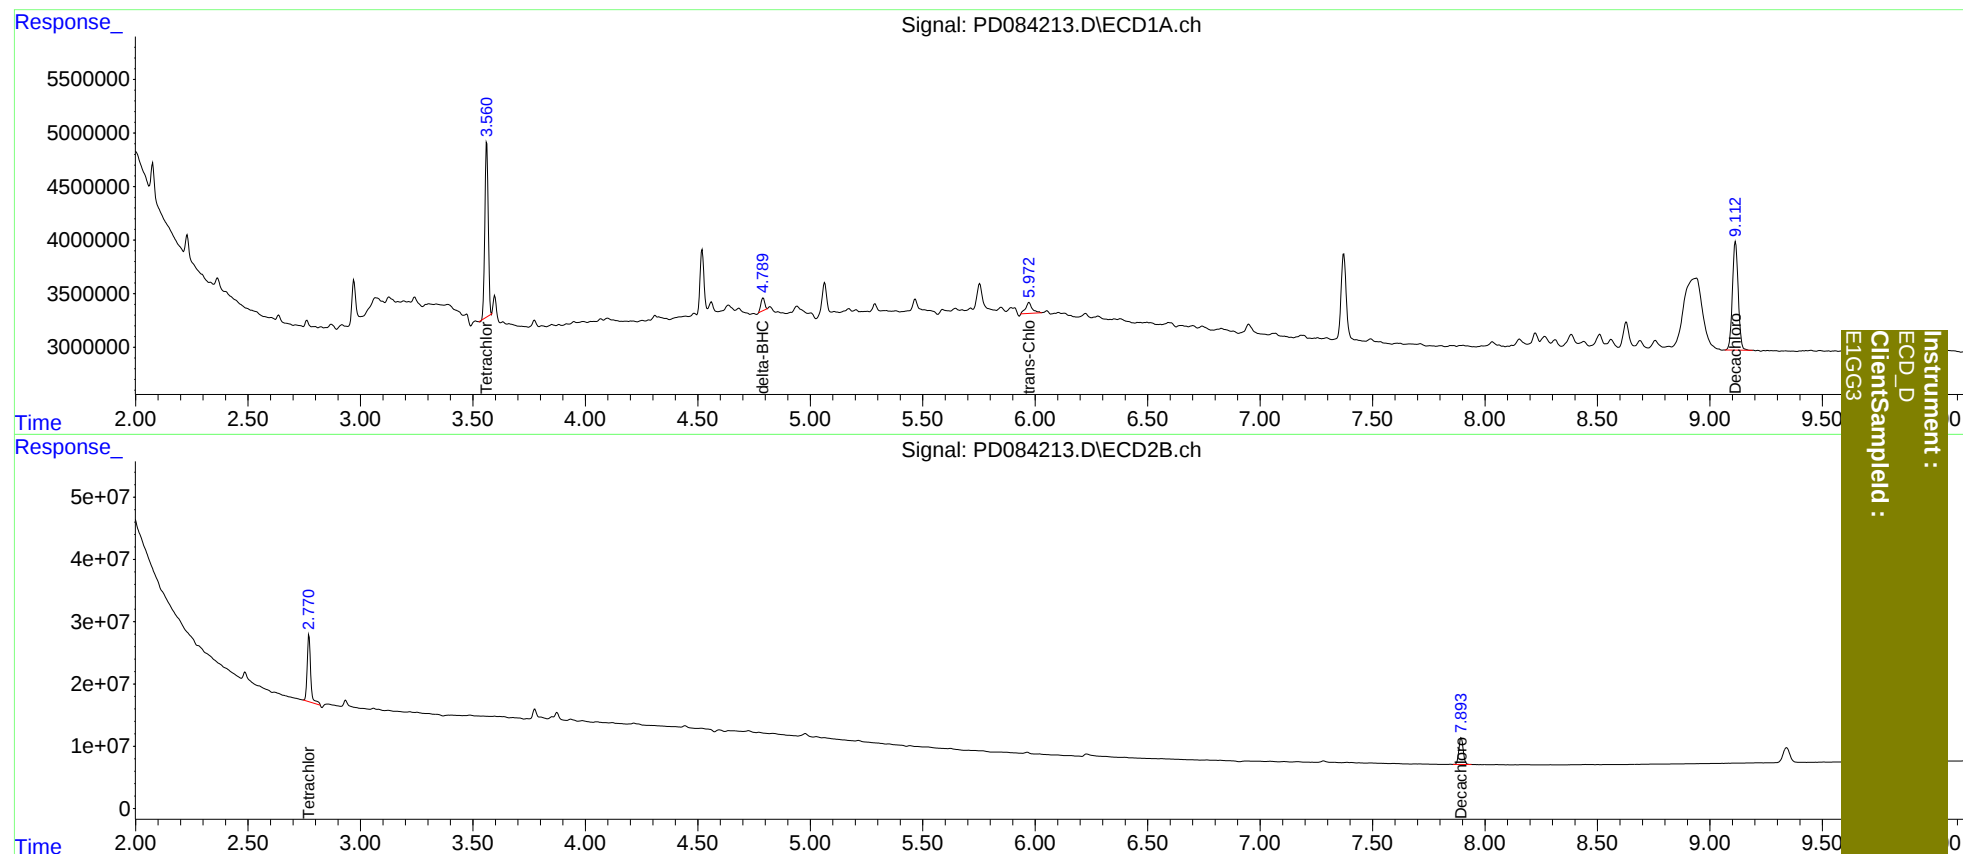


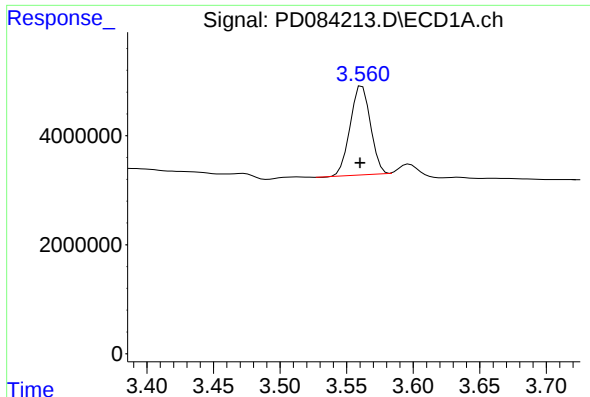

#1 Tetrachloro-m-xylene


R.T.: 3.562 min
Delta R.T.: 0.002 min
Response: 17276096
Conc: 19.29 ng/ml

Instrument :
ECD_D
ClientSampleId :
E1GG3

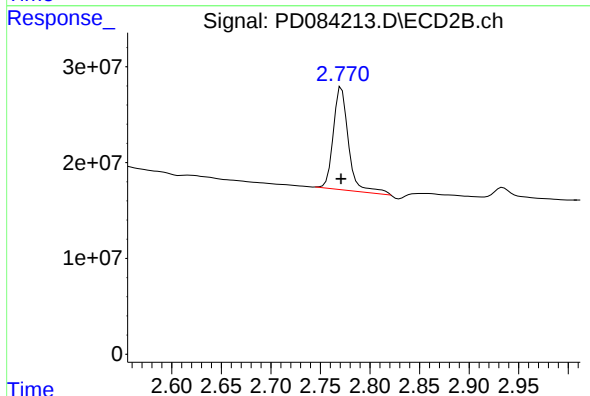


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: 0.000 min
Response: 114435966
Conc: 21.94 ng/ml

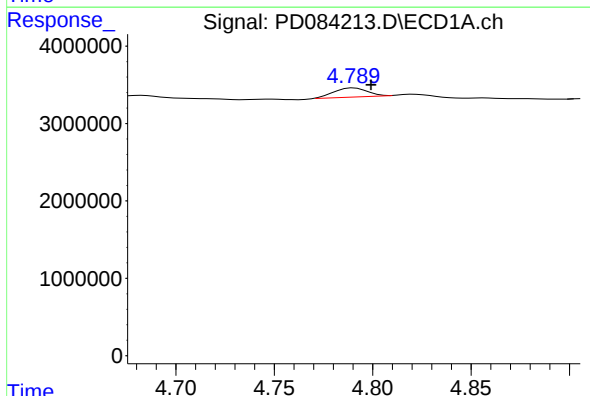


#7 delta-BHC

R.T.: 4.790 min
Delta R.T.: -0.009 min
Response: 1381214
Conc: 0.69 ng/ml

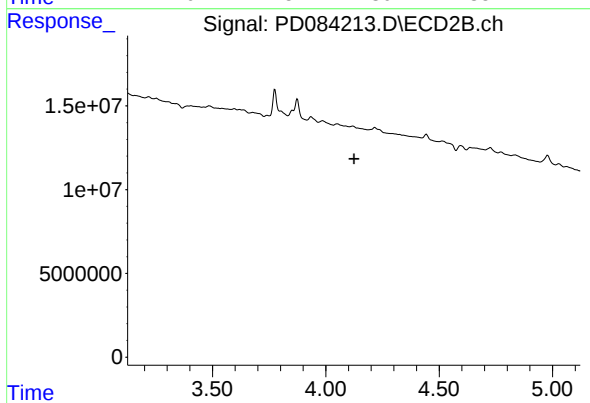

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.124 min
Response: 0
Conc: N.D.

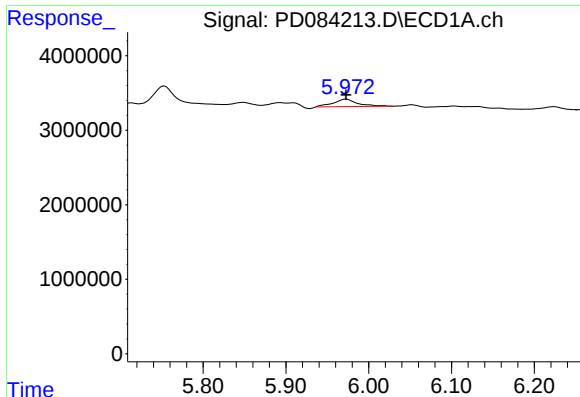

#10 trans-Chlordane


R.T.: 5.973 min
Delta R.T.: 0.000 min
Response: 2094927
Conc: 1.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
E1GG3

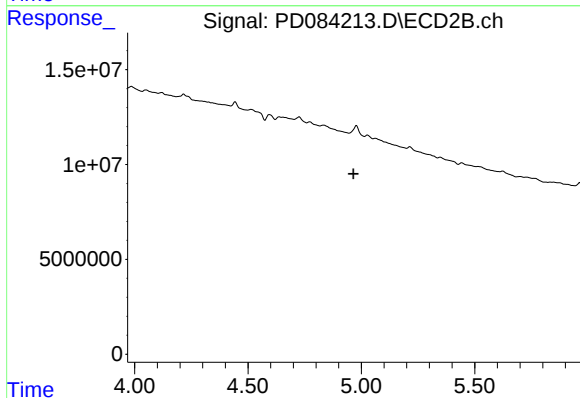


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.965 min
Response: 0
Conc: N.D.

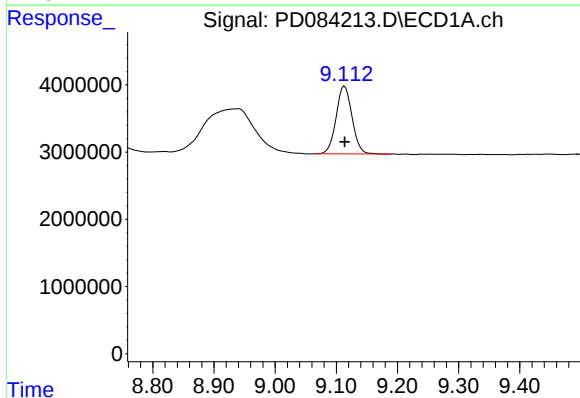

#27 Decachlorobiphenyl

R.T.: 9.114 min
Delta R.T.: 0.000 min
Response: 18184010
Conc: 9.47 ng/ml

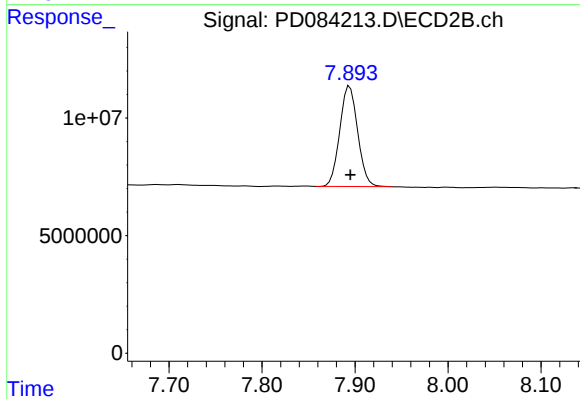

#27 Decachlorobiphenyl

R.T.: 7.894 min
Delta R.T.: 0.000 min
Response: 57248487
Conc: 9.93 ng/ml