

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080524\
 Data File : PD084214.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Aug 2024 11:13
 Operator : AR\AJ
 Sample : P3401-04MS
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E1GG3MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/06/2024
 Supervised By :Ankita Jodhani 08/06/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 01:18:27 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072424CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 25 11:17:53 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.562	2.771	16848906	105.5E6	18.818	20.227
27)	SA Decachlor...	9.114	7.895	18431189	58889661	9.603	10.215
Target Compounds							
2)	A alpha-BHC	4.019	3.270	90913372	445.7E6	54.641	52.133
3)	MA gamma-BHC...	4.353	3.599	90668426	412.7E6	54.887	52.603
4)	MA Heptachlor	4.945	3.936	91786064	373.7E6	49.966	48.193
5)	MB Aldrin	5.288	4.215	91002102	388.8E6	49.285	49.387
6)	B beta-BHC	4.549	3.894	37372900	160.0E6	50.004m	44.768m
7)	B delta-BHC	4.799	4.124	93963487	421.9E6	46.863	49.532
8)	B Heptachlo...	5.716	4.716	84142944	352.7E6	45.520	48.630
9)	A Endosulfan I	6.103	5.085	86570187	332.5E6	50.099	51.441
10)	B trans-Chl...	5.973	4.965	89924624	365.6E6	50.677	51.615
11)	B cis-Chlor...	6.052	5.029	89510203	356.6E6	49.057	49.334
12)	B 4,4'-DDE	6.225	5.217	177.5E6	676.4E6	96.519	98.453
13)	MA Dieldrin	6.379	5.349	193.7E6	715.1E6	104.000	100.909
14)	MA Endrin	6.611	5.624	160.2E6	602.8E6	100.483	98.843
15)	B Endosulfa...	6.830	5.918	169.3E6	588.3E6	96.370	97.993
16)	A 4,4'-DDD	6.744	5.770	136.8E6	526.4E6	104.307	100.604
17)	MA 4,4'-DDT	7.060	6.021	145.4E6	527.7E6	102.693	101.045
18)	B Endrin al...	6.961	6.097	129.2E6	450.9E6	103.033	101.898
19)	B Endosulfa...	7.196	6.320	162.9E6	576.3E6	100.145	100.400
20)	A Methoxychlor	7.536	6.595	384.4E6	1076.7E6	457.352	417.370
21)	B Endrin ke...	7.683	6.825	184.4E6	635.9E6	102.359	102.139

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080524\
Data File : PD084214.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Aug 2024 11:13
Operator : AR\AJ
Sample : P3401-04MS
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 01:18:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072424CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 25 11:17:53 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

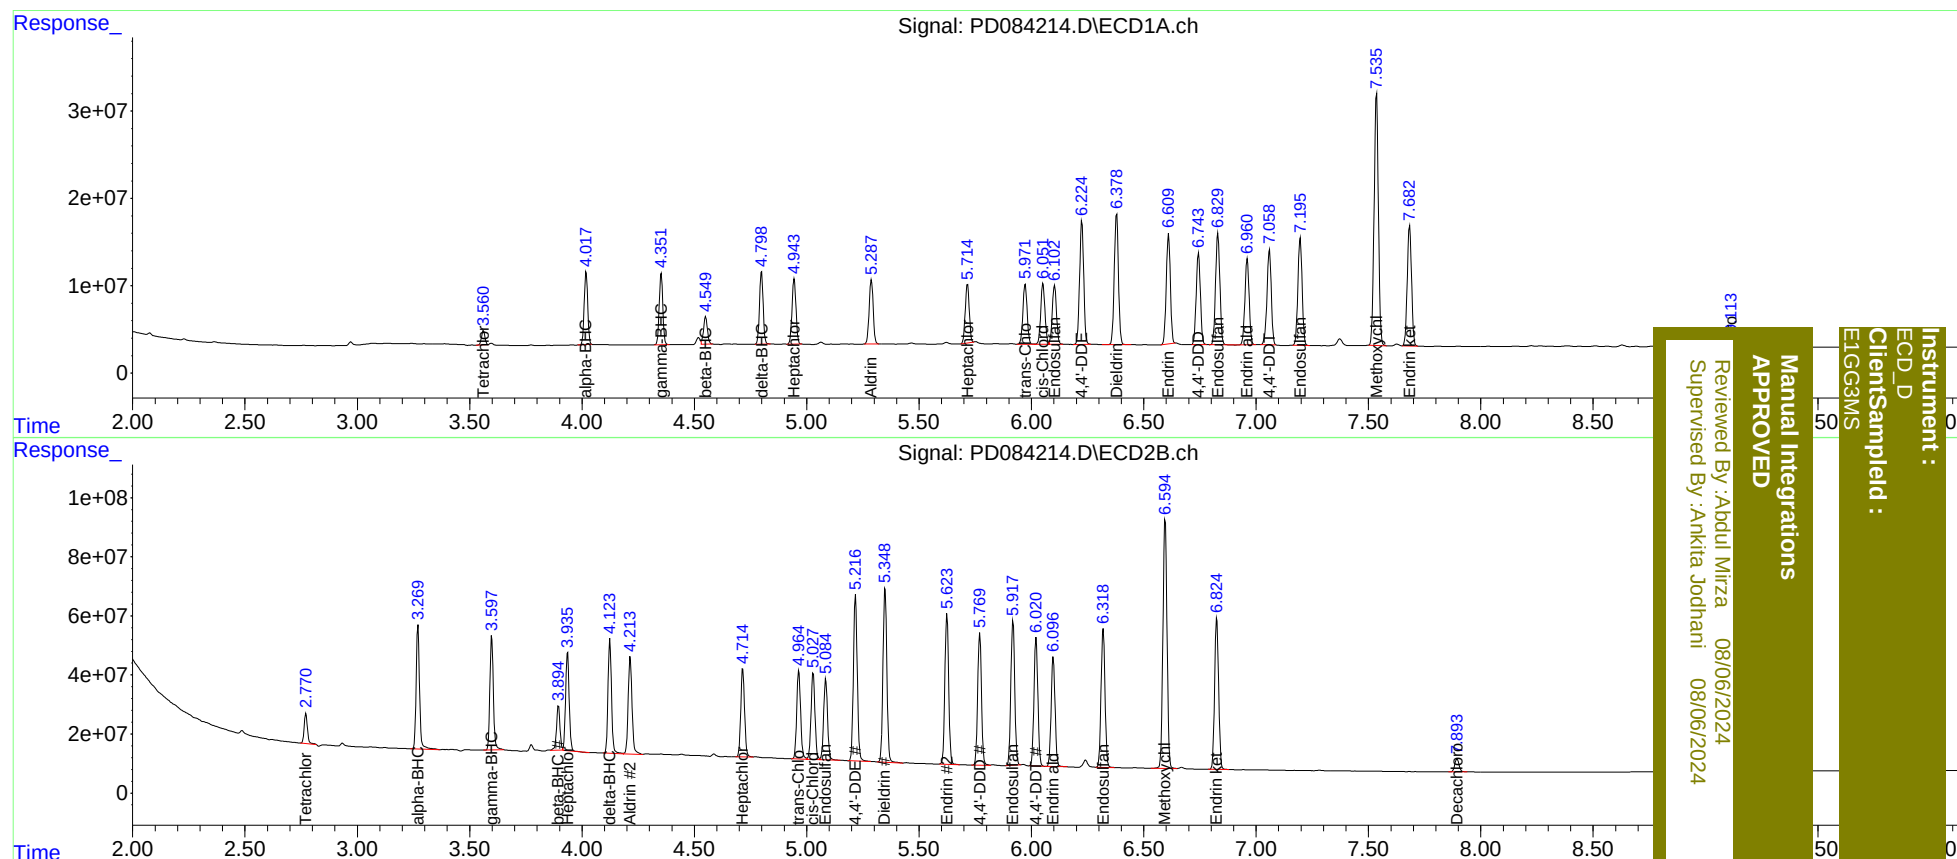

Instrument :
ECD_D
ClientSampled :
E1GG3MS

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 08/06/2024
Supervised By: Ankita Jodhani 08/06/2024