

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080524\
 Data File : PD084215.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Aug 2024 11:26
 Operator : AR\AJ
 Sample : P3401-05MSD
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E1GG3MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/06/2024
 Supervised By :Ankita Jodhani 08/06/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 01:18:44 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072424CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 25 11:17:53 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.561	2.771	16957635	107.8E6	18.939	20.661
2)	SA Decachlor...	9.115	7.895	18627696	58996984	9.705	10.234
Target Compounds							
2)	A alpha-BHC	4.019	3.270	91584505	445.6E6	55.044	52.126
3)	MA gamma-BHC...	4.353	3.598	90712923	412.2E6	54.914	52.547
4)	MA Heptachlor	4.945	3.936	91981080	376.1E6	50.072	48.493
5)	MB Aldrin	5.288	4.215	91003277	386.8E6	49.285	49.134
6)	B beta-BHC	4.549	3.894	37084417	158.5E6	49.618m	44.354m
7)	B delta-BHC	4.799	4.124	94143435	422.0E6	46.953	49.535
8)	B Heptachlo...	5.716	4.716	84230907	352.6E6	45.568	48.613
9)	A Endosulfan I	6.103	5.085	86726375	332.6E6	50.189	51.453
10)	B trans-Chl...	5.973	4.965	89969881	365.0E6	50.702	51.536
11)	B cis-Chlor...	6.052	5.029	89352779	356.1E6	48.971	49.257
12)	B 4,4'-DDE	6.225	5.217	177.5E6	674.8E6	96.488	98.220
13)	MA Dieldrin	6.379	5.349	193.8E6	715.2E6	104.063	100.925
14)	MA Endrin	6.611	5.624	160.6E6	605.8E6	100.752	99.342
15)	B Endosulfa...	6.830	5.918	169.7E6	588.6E6	96.564	98.037
16)	A 4,4'-DDD	6.744	5.771	137.1E6	527.5E6	104.536	100.819
17)	MA 4,4'-DDT	7.059	6.021	146.4E6	528.5E6	103.348	101.201
18)	B Endrin al...	6.961	6.098	129.2E6	451.2E6	103.017	101.974
19)	B Endosulfa...	7.196	6.320	163.7E6	576.8E6	100.612	100.481
20)	A Methoxychlor	7.535	6.596	387.8E6	1086.0E6	461.375	420.979
21)	B Endrin ke...	7.683	6.826	185.0E6	637.6E6	102.646	102.409

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080524\
Data File : PD084215.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Aug 2024 11:26
Operator : AR\AJ
Sample : P3401-05MSD
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 01:18:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072424CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 25 11:17:53 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

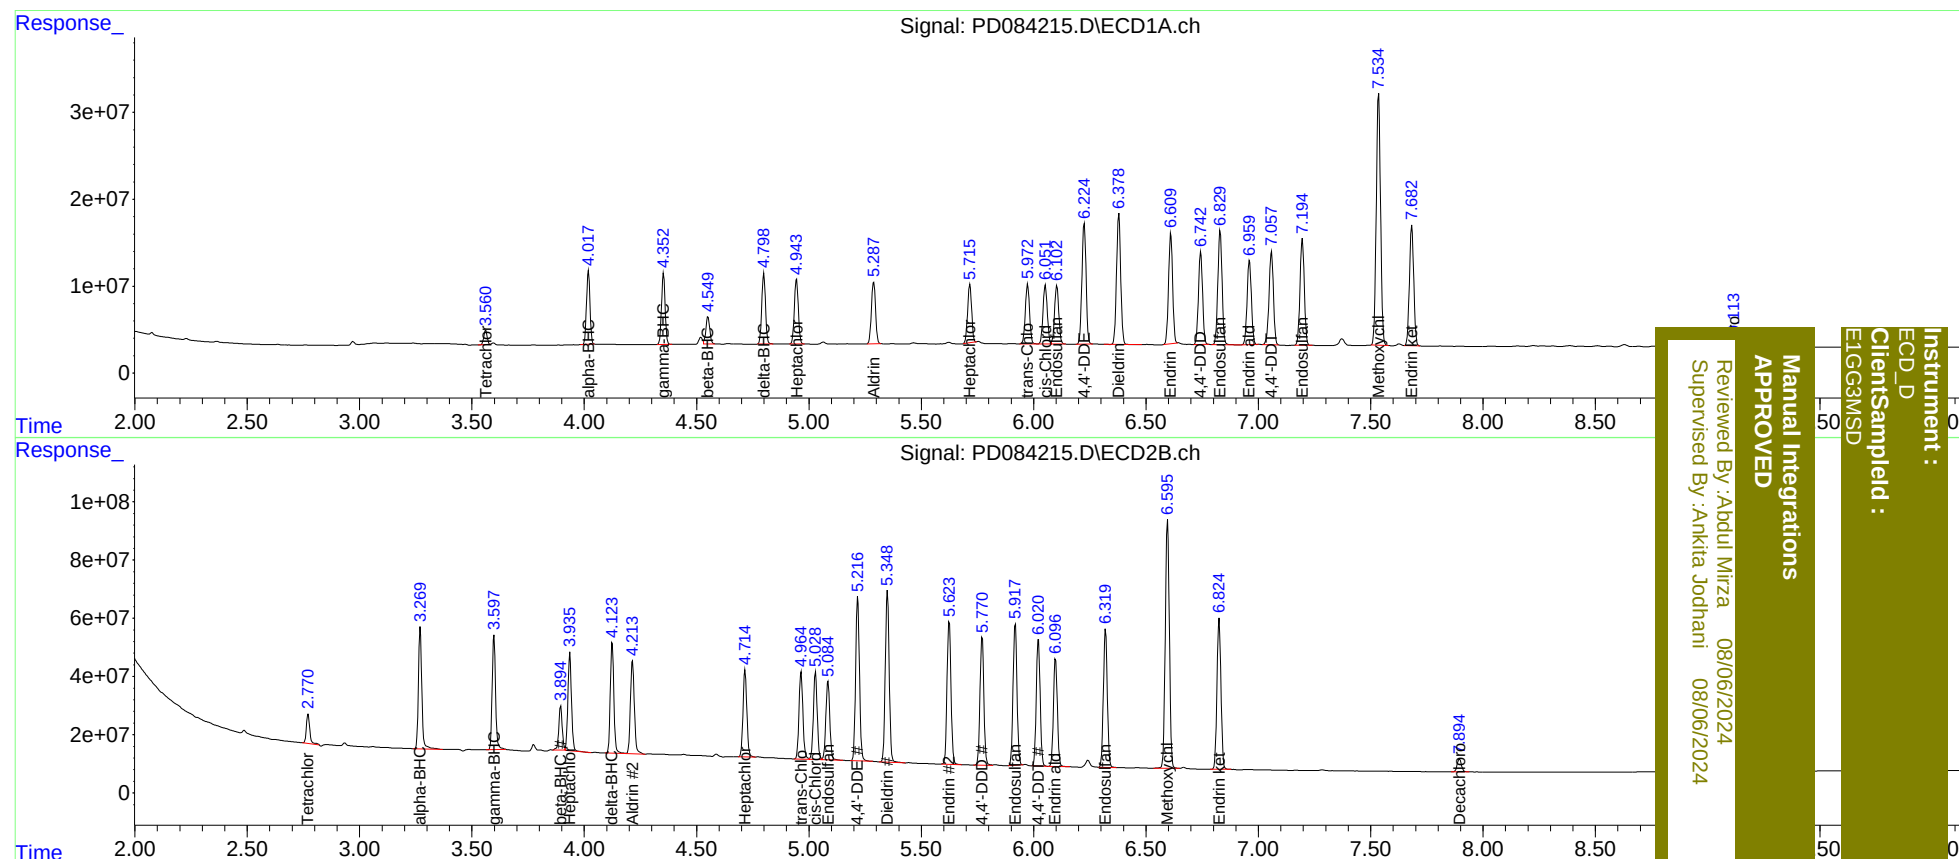

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 08/06/2024
Supervised By: Ankita Jodhani 08/06/2024

Instrument :
ECD_D
Client Sampled :
E1GG3MSD