

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080525\
 Data File : PD089741.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Aug 2025 12:27
 Operator : AR\AJ
 Sample : Q2744-11
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 05 22:08:44 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071725CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 18 07:15:53 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds


3) MA	gamma-BHC...	4.344	0.000	195608	0	<MDL	N.D.	#
7) B	delta-BHC	4.781	0.000	184727	0	<MDL	N.D.	#
8) B	Heptachlo...	5.685	0.000	1940035	0	0.394	N.D.	#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080525\
Data File : PD089741.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Aug 2025 12:27
Operator : AR\AJ
Sample : Q2744-11
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 05 22:08:44 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071725CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 18 07:15:53 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

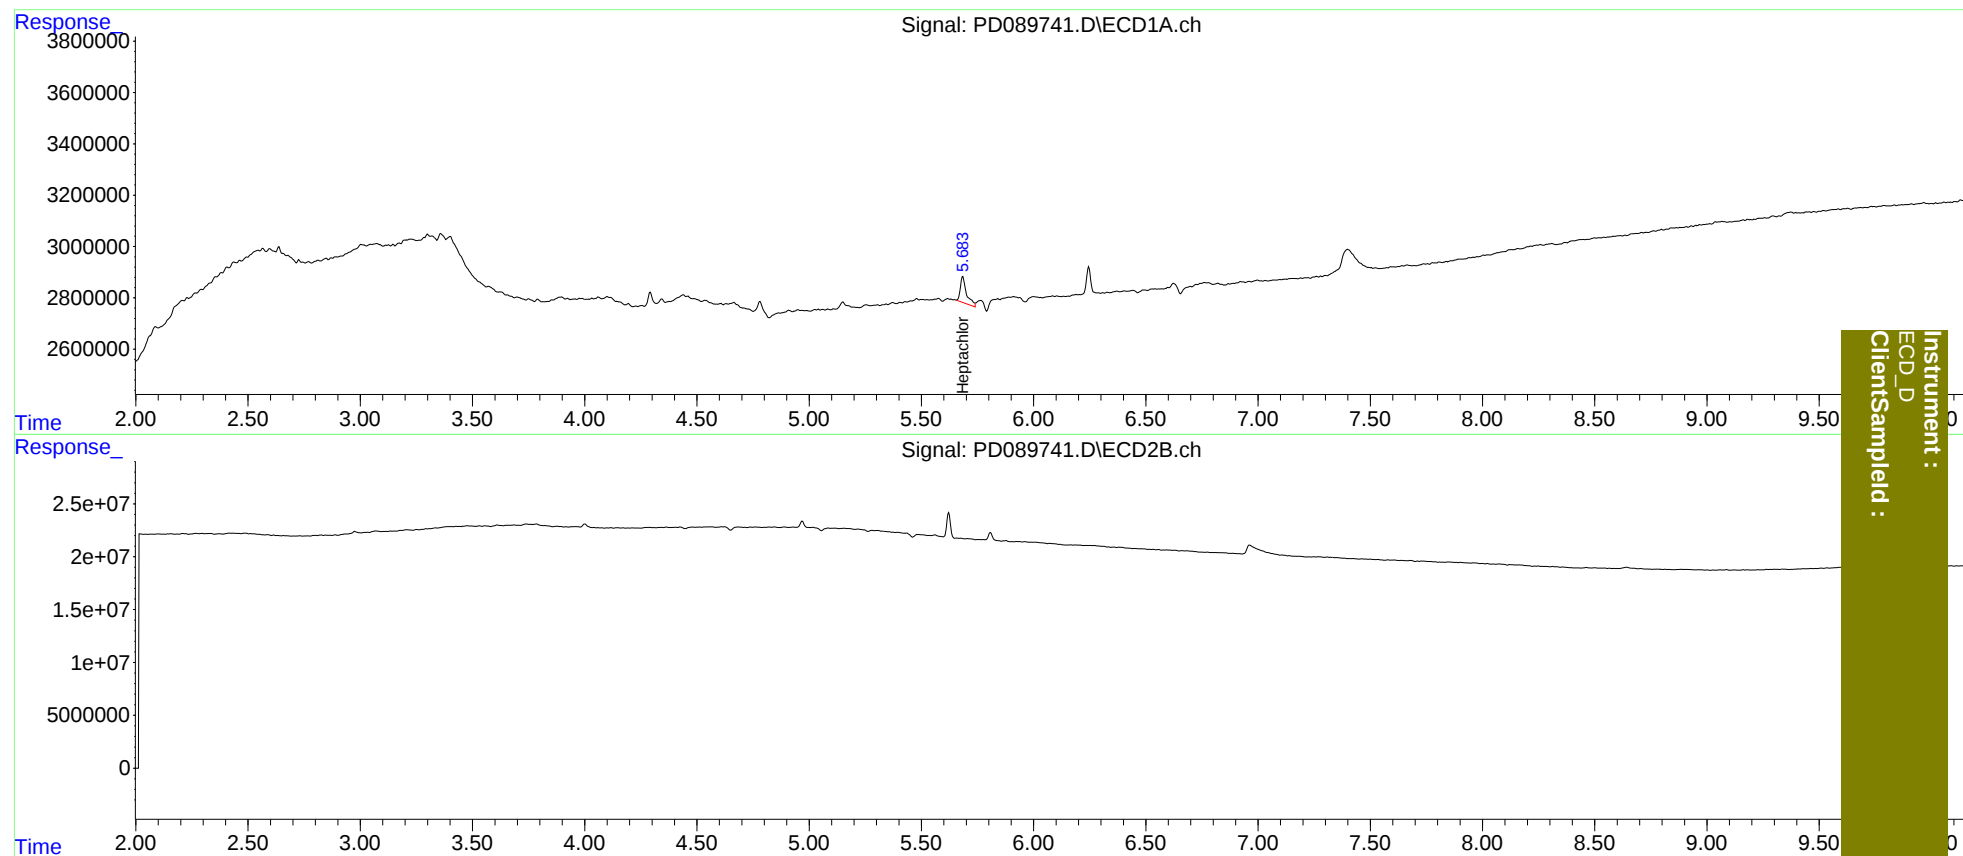


Instrument :
ECD_D
ClientSampled :
0

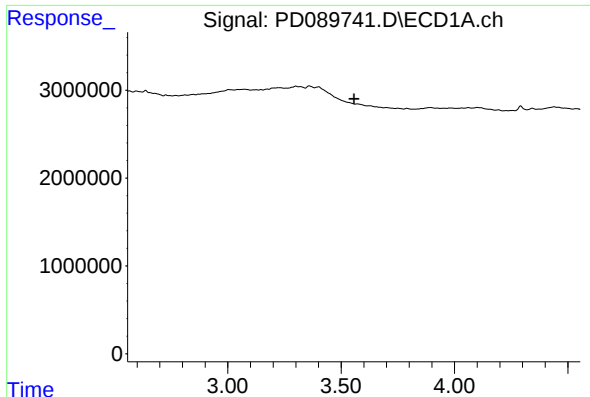

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.557 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

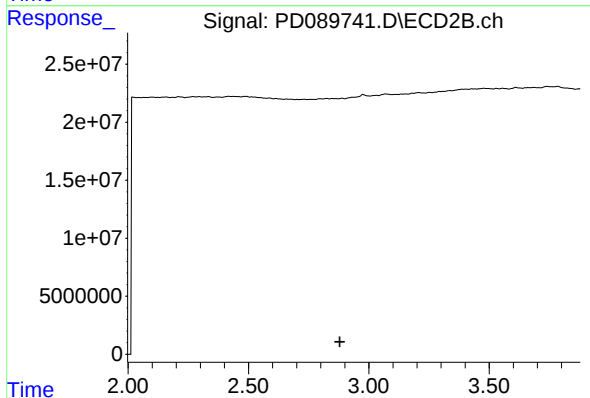


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 2.879 min
Response: 0
Conc: N.D.

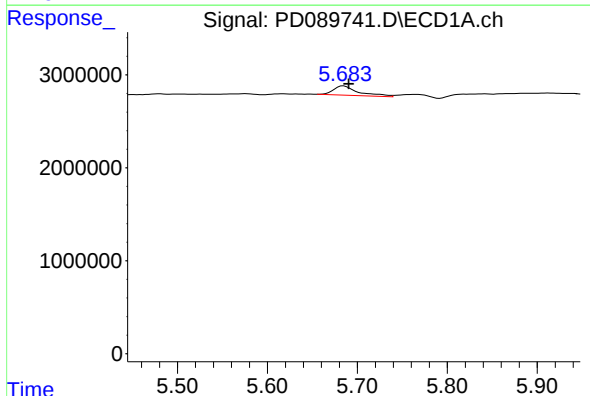


#8 Heptachlor epoxide

R.T.: 5.685 min
Delta R.T.: -0.006 min
Response: 1940035
Conc: 0.39 ng/ml

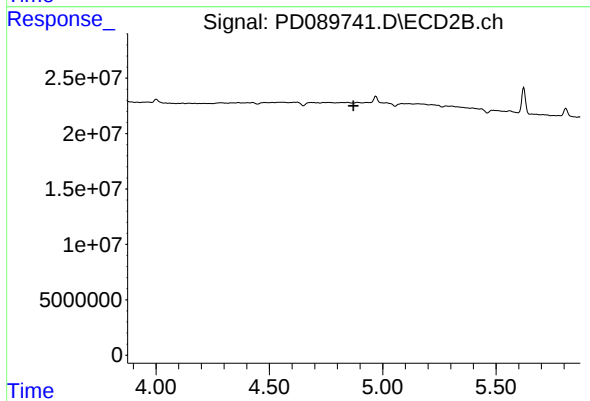

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.871 min
Response: 0
Conc: N.D.

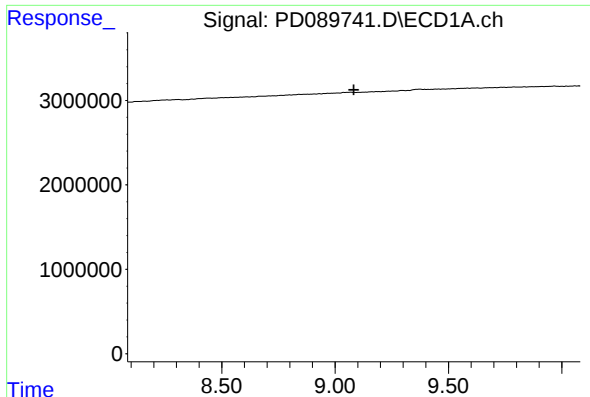

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.082 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

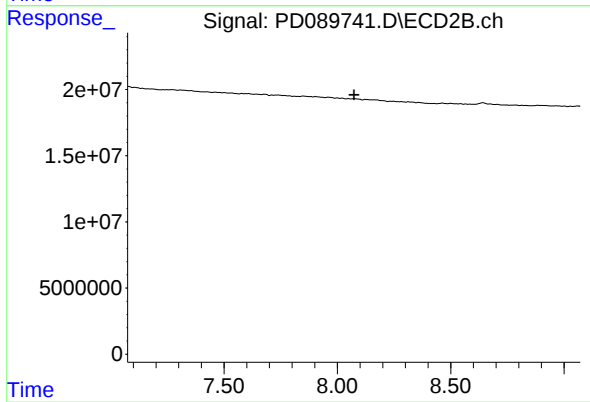

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.074 min
Response: 0
Conc: N.D.