

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080620\
 Data File : PD058876.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2020 07:26
 Operator : DD\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 09:40:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 06 09:11:39 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.207	3.865	4923851	7320958	5.029	4.930
27)	SA Decachlor...	7.840	8.859	11494843	15801658	10.798	11.548
Target Compounds							
2)	A alpha-BHC	3.629	4.247	6649018	9998367	4.679	4.773
3)	MA gamma-BHC...	3.899	4.528	7338353	9150049	5.342	4.689
4)	MA Heptachlor	4.178	5.028	6000663	9569753	5.049	5.065
9)	A Endosulfan I	5.172	6.063	5535481	7996634	5.050	5.080
13)	MA Dieldrin	5.409	6.319	11840631	16538901	9.707	9.796
14)	MA Endrin	5.660	6.534	10258754	13809783	10.594	10.157
16)	A 4,4'-DDD	5.798	6.663	9115685	12689693	9.667	9.532
17)	MA 4,4'-DDT	6.031	6.960	8404191	12466456	9.288	9.470
20)	A Methoxychlor	6.579	7.420	23088144	38176692	51.063	55.055


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080620\
Data File : PD058876.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2020 07:26
Operator : DD\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 09:40:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 06 09:11:39 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

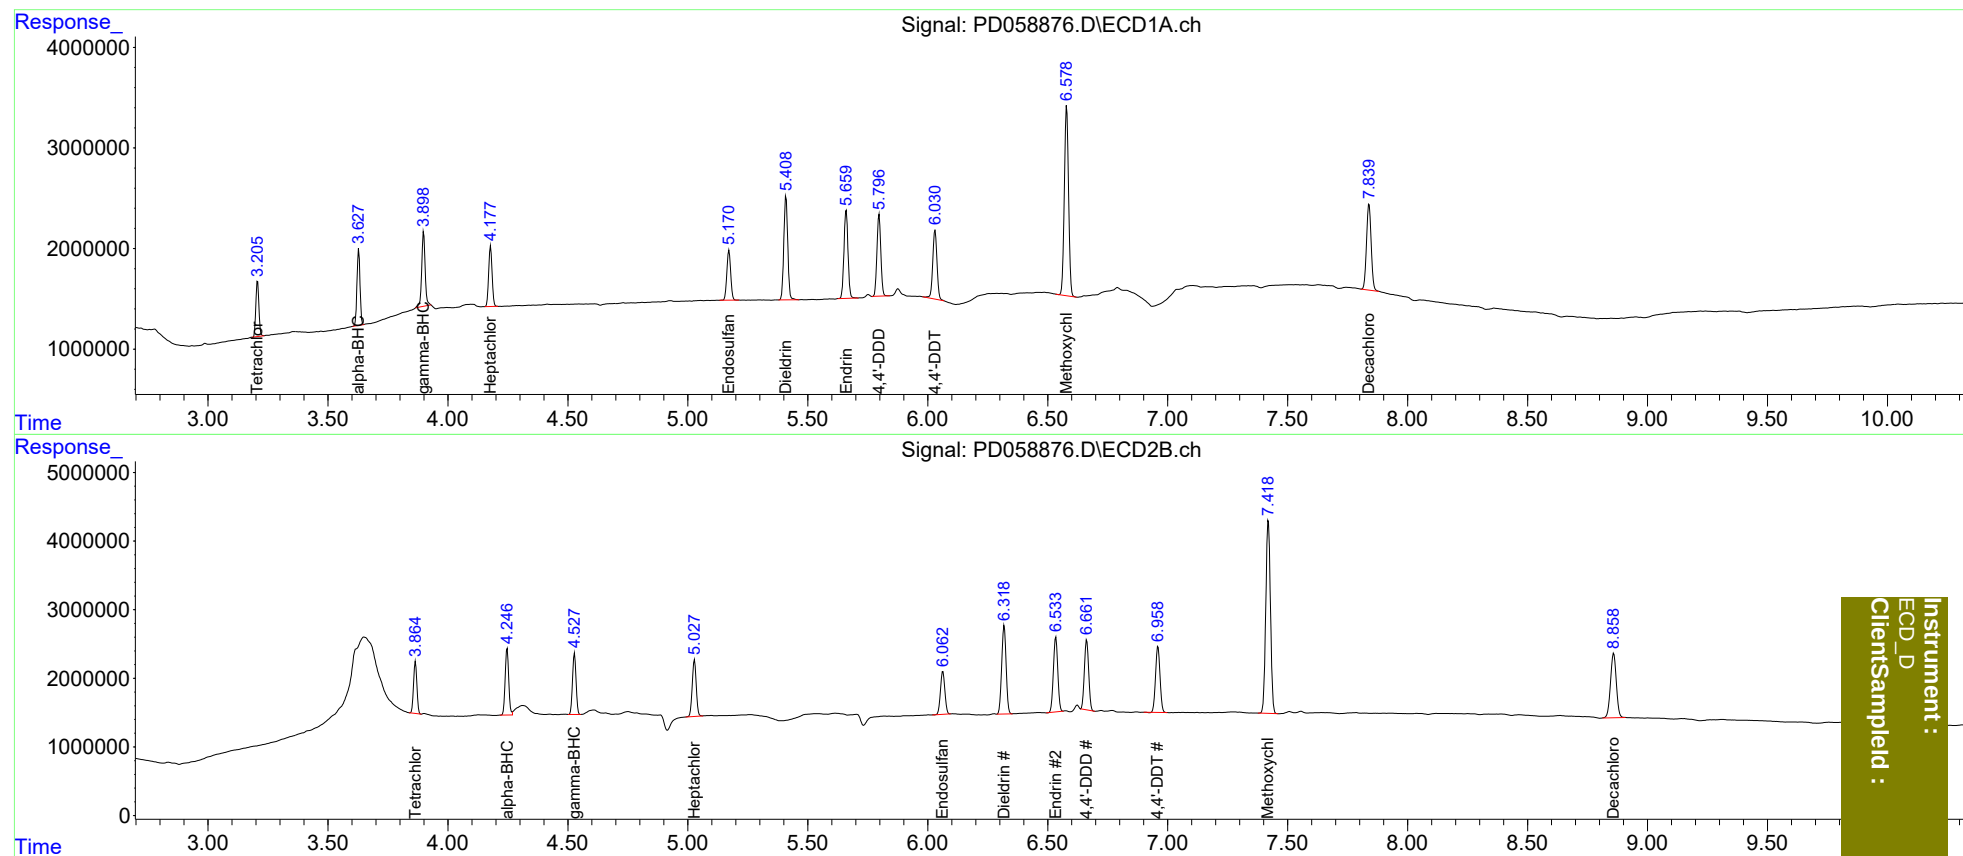


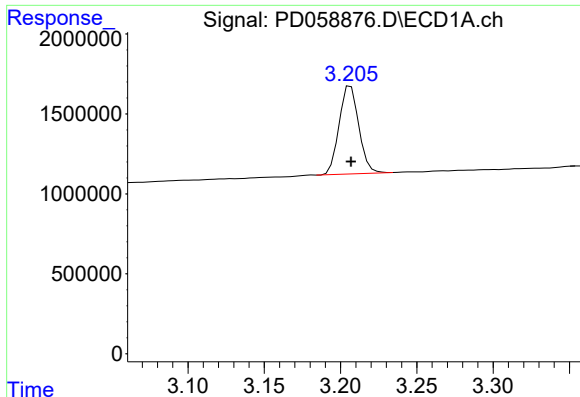

#1 Tetrachloro-m-xylene


R.T.: 3.207 min
Delta R.T.: 0.000 min
Response: 4923851
Conc: 5.03 ng/ml

Instrument :
ECD_D
ClientSampleId :

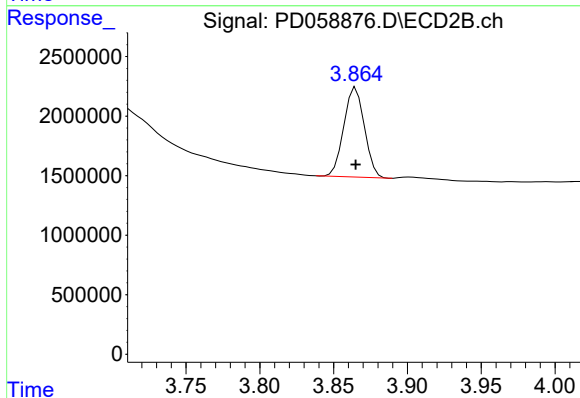


#1 Tetrachloro-m-xylene

R.T.: 3.865 min
Delta R.T.: 0.000 min
Response: 7320958
Conc: 4.93 ng/ml

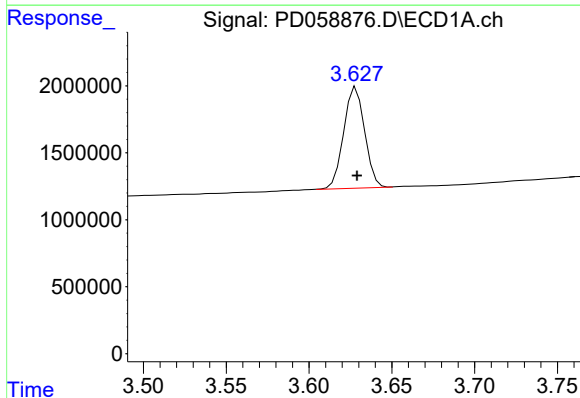


#2 alpha-BHC

R.T.: 3.629 min
Delta R.T.: 0.000 min
Response: 6649018
Conc: 4.68 ng/ml

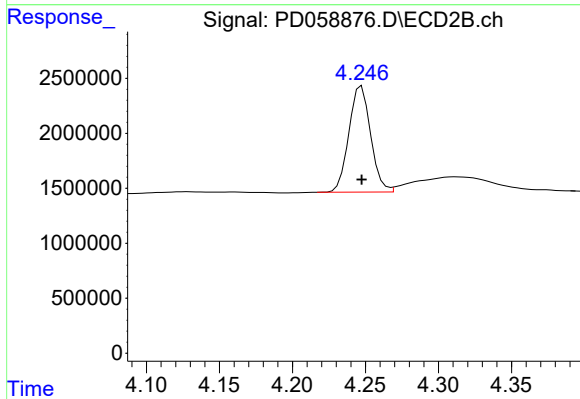

#2 alpha-BHC


R.T.: 4.247 min
Delta R.T.: 0.000 min
Response: 9998367
Conc: 4.77 ng/ml

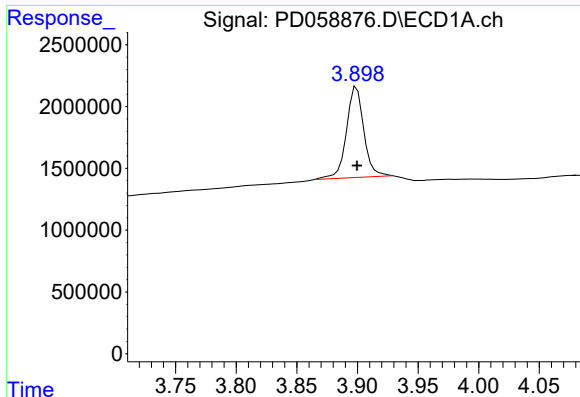

#3 gamma-BHC (Lindane)


R.T.: 3.899 min
Delta R.T.: 0.000 min
Response: 7338353
Conc: 5.34 ng/ml

Instrument :
ECD_D
ClientSampleId :

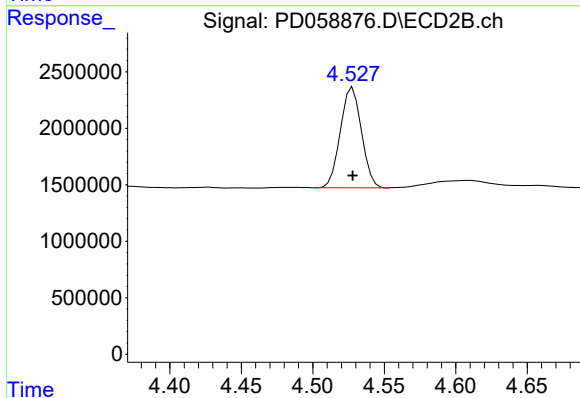


#3 gamma-BHC (Lindane)

R.T.: 4.528 min
Delta R.T.: 0.000 min
Response: 9150049
Conc: 4.69 ng/ml

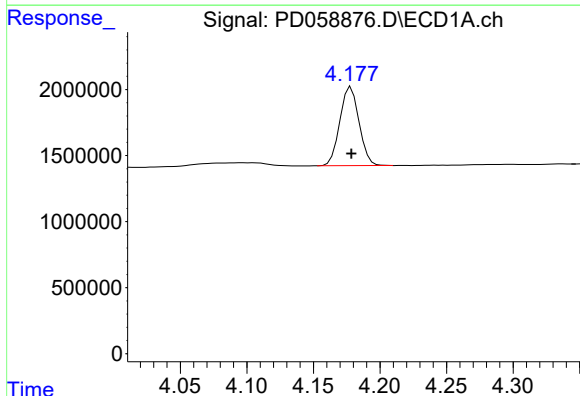


#4 Heptachlor

R.T.: 4.178 min
Delta R.T.: 0.000 min
Response: 6000663
Conc: 5.05 ng/ml

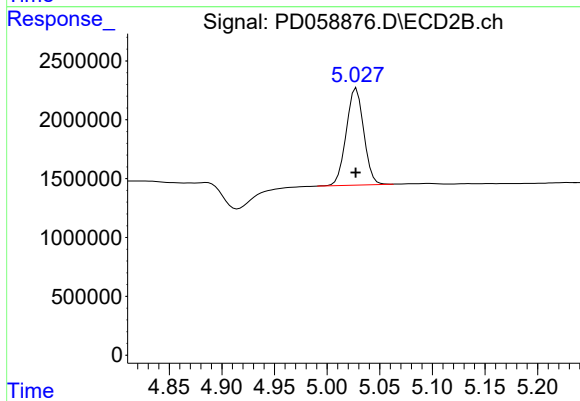

#4 Heptachlor


R.T.: 5.028 min
Delta R.T.: 0.000 min
Response: 9569753
Conc: 5.07 ng/ml

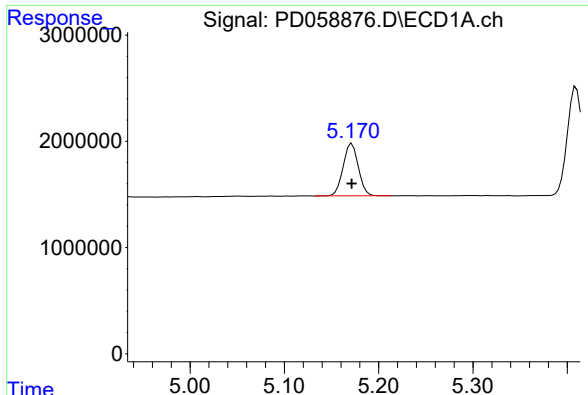

#9 Endosulfan I


R.T.: 5.172 min
Delta R.T.: 0.000 min
Response: 5535481
Conc: 5.05 ng/ml

Instrument :
ECD_D
ClientSampleId :

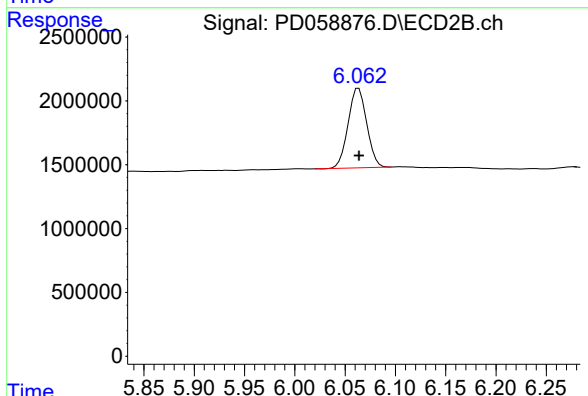


#9 Endosulfan I

R.T.: 6.063 min
Delta R.T.: 0.000 min
Response: 7996634
Conc: 5.08 ng/ml

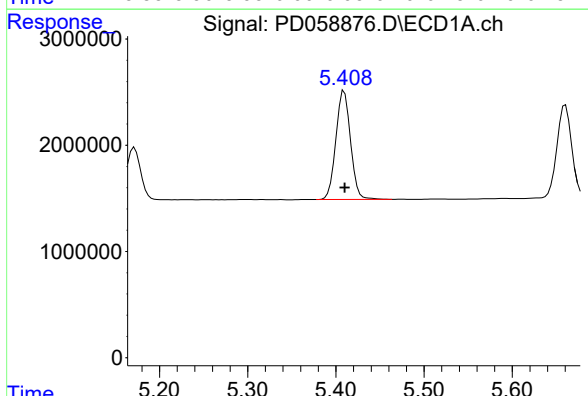


#13 Dieldrin

R.T.: 5.409 min
Delta R.T.: 0.000 min
Response: 11840631
Conc: 9.71 ng/ml

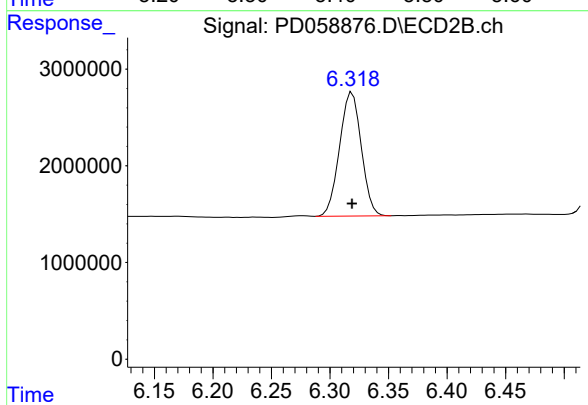

#13 Dieldrin


R.T.: 6.319 min
Delta R.T.: 0.000 min
Response: 16538901
Conc: 9.80 ng/ml

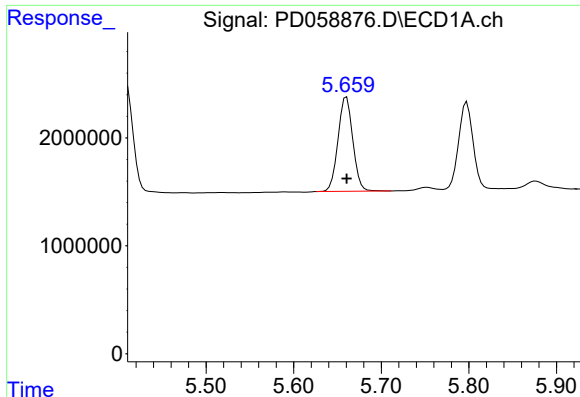

#14 Endrin


R.T.: 5.660 min
Delta R.T.: 0.000 min
Response: 10258754
Conc: 10.59 ng/ml

Instrument :
ECD_D
ClientSampleId :

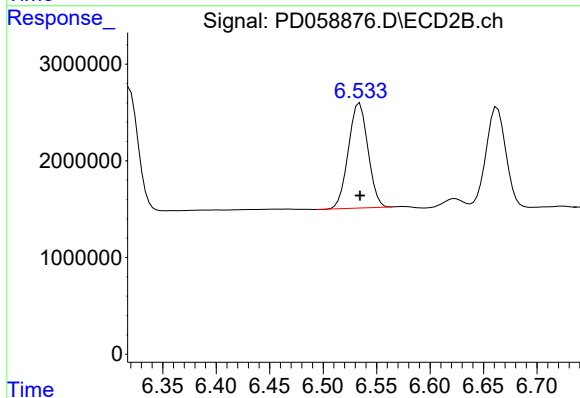


#14 Endrin

R.T.: 6.534 min
Delta R.T.: 0.000 min
Response: 13809783
Conc: 10.16 ng/ml

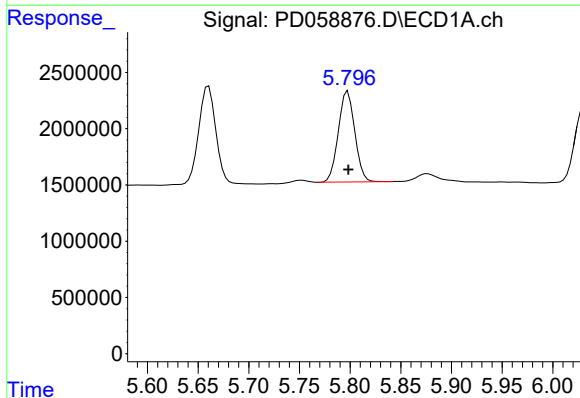


#16 4,4'-DDD

R.T.: 5.798 min
Delta R.T.: 0.000 min
Response: 9115685
Conc: 9.67 ng/ml

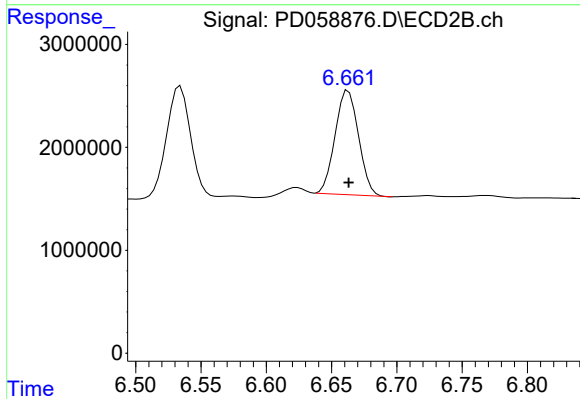

#16 4,4'-DDD


R.T.: 6.663 min
Delta R.T.: 0.000 min
Response: 12689693
Conc: 9.53 ng/ml

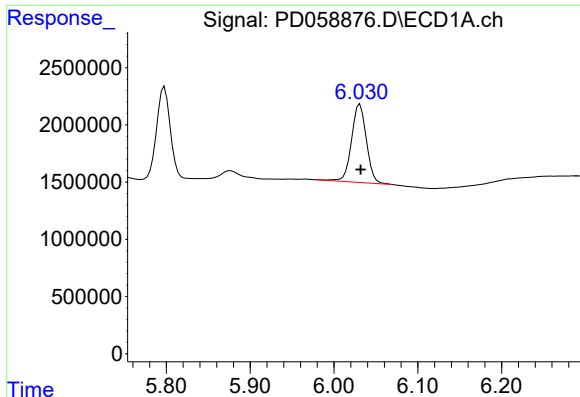

#17 4,4'-DDT


R.T.: 6.031 min
Delta R.T.: 0.000 min
Response: 8404191
Conc: 9.29 ng/ml

Instrument :
ECD_D
ClientSampleId :

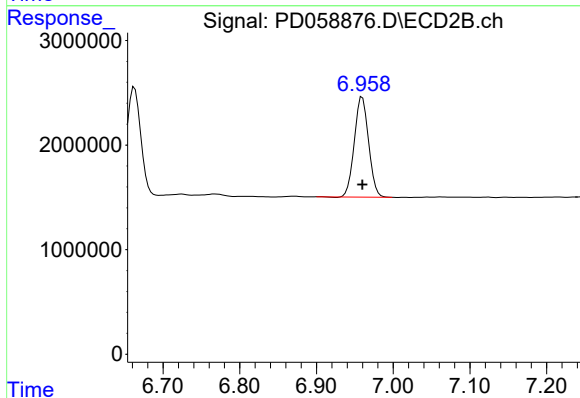


#17 4,4'-DDT

R.T.: 6.960 min
Delta R.T.: 0.000 min
Response: 12466456
Conc: 9.47 ng/ml

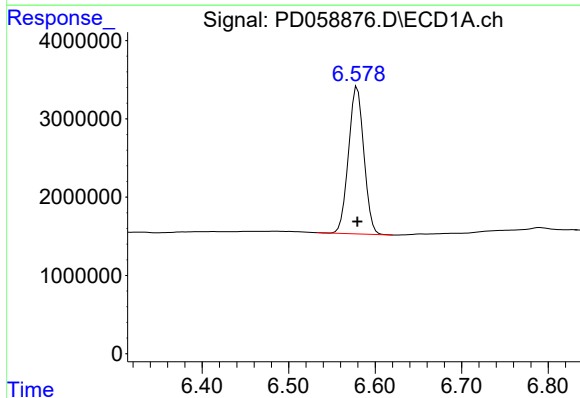


#20 Methoxychlor

R.T.: 6.579 min
Delta R.T.: 0.000 min
Response: 23088144
Conc: 51.06 ng/ml

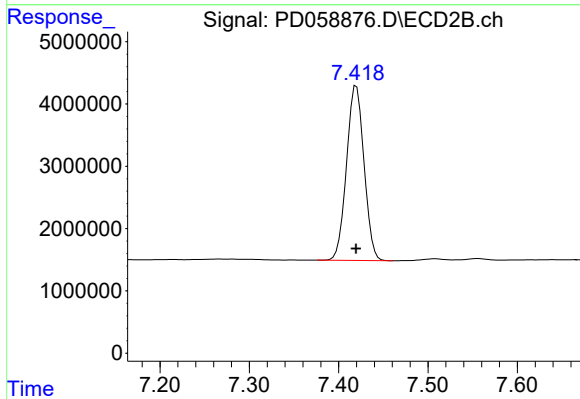

#20 Methoxychlor


R.T.: 7.420 min
Delta R.T.: 0.000 min
Response: 38176692
Conc: 55.05 ng/ml

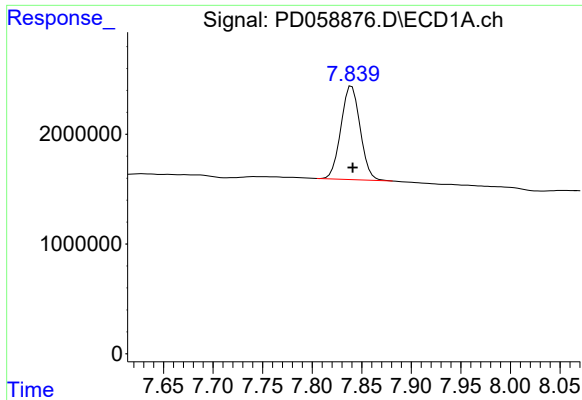

#27 Decachlorobiphenyl

R.T.: 7.840 min
Delta R.T.: 0.000 min
Response: 11494843
Conc: 10.80 ng/ml

Instrument :
ECD_D
ClientSampleId :

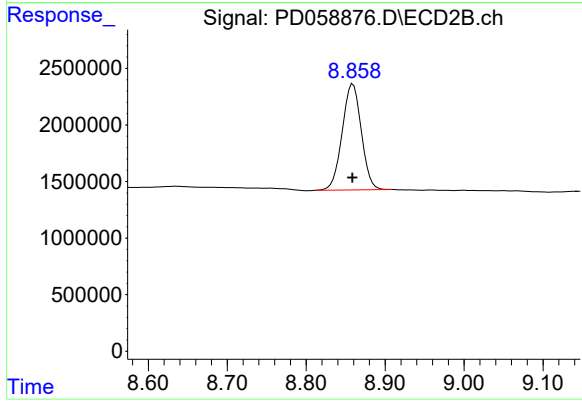

#27 Decachlorobiphenyl

R.T.: 8.859 min
Delta R.T.: 0.000 min
Response: 15801658
Conc: 11.55 ng/ml