

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080620\
 Data File : PD058878.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2020 07:54
 Operator : DD\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 09:40:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 06 09:11:39 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.207	3.865	9951436	14697705	10.163	9.898
27)	SA Decachlor...	7.840	8.859	22230746	29726113	20.883	21.724
Target Compounds							
2)	A alpha-BHC	3.628	4.247	13733920	20410197	9.666	9.744
3)	MA gamma-BHC...	3.899	4.527	13882924	18761655	10.106	9.614
4)	MA Heptachlor	4.178	5.027	12020511	18887001	10.114	9.996
9)	A Endosulfan I	5.172	6.064	11160455	15949558	10.181	10.132
13)	MA Dieldrin	5.409	6.319	24080190	33638396	19.740	19.924
14)	MA Endrin	5.661	6.534	20414933	26315693	21.082	19.355
16)	A 4,4'-DDD	5.798	6.663	14544108	26017690	15.423	19.543 #
17)	MA 4,4'-DDT	6.032	6.960	17244552	26096171	19.057	19.824
20)	A Methoxychlor	6.580	7.420	46988791	70514499	103.923	101.689

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080620\
Data File : PD058878.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2020 07:54
Operator : DD\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 09:40:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 06 09:11:39 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

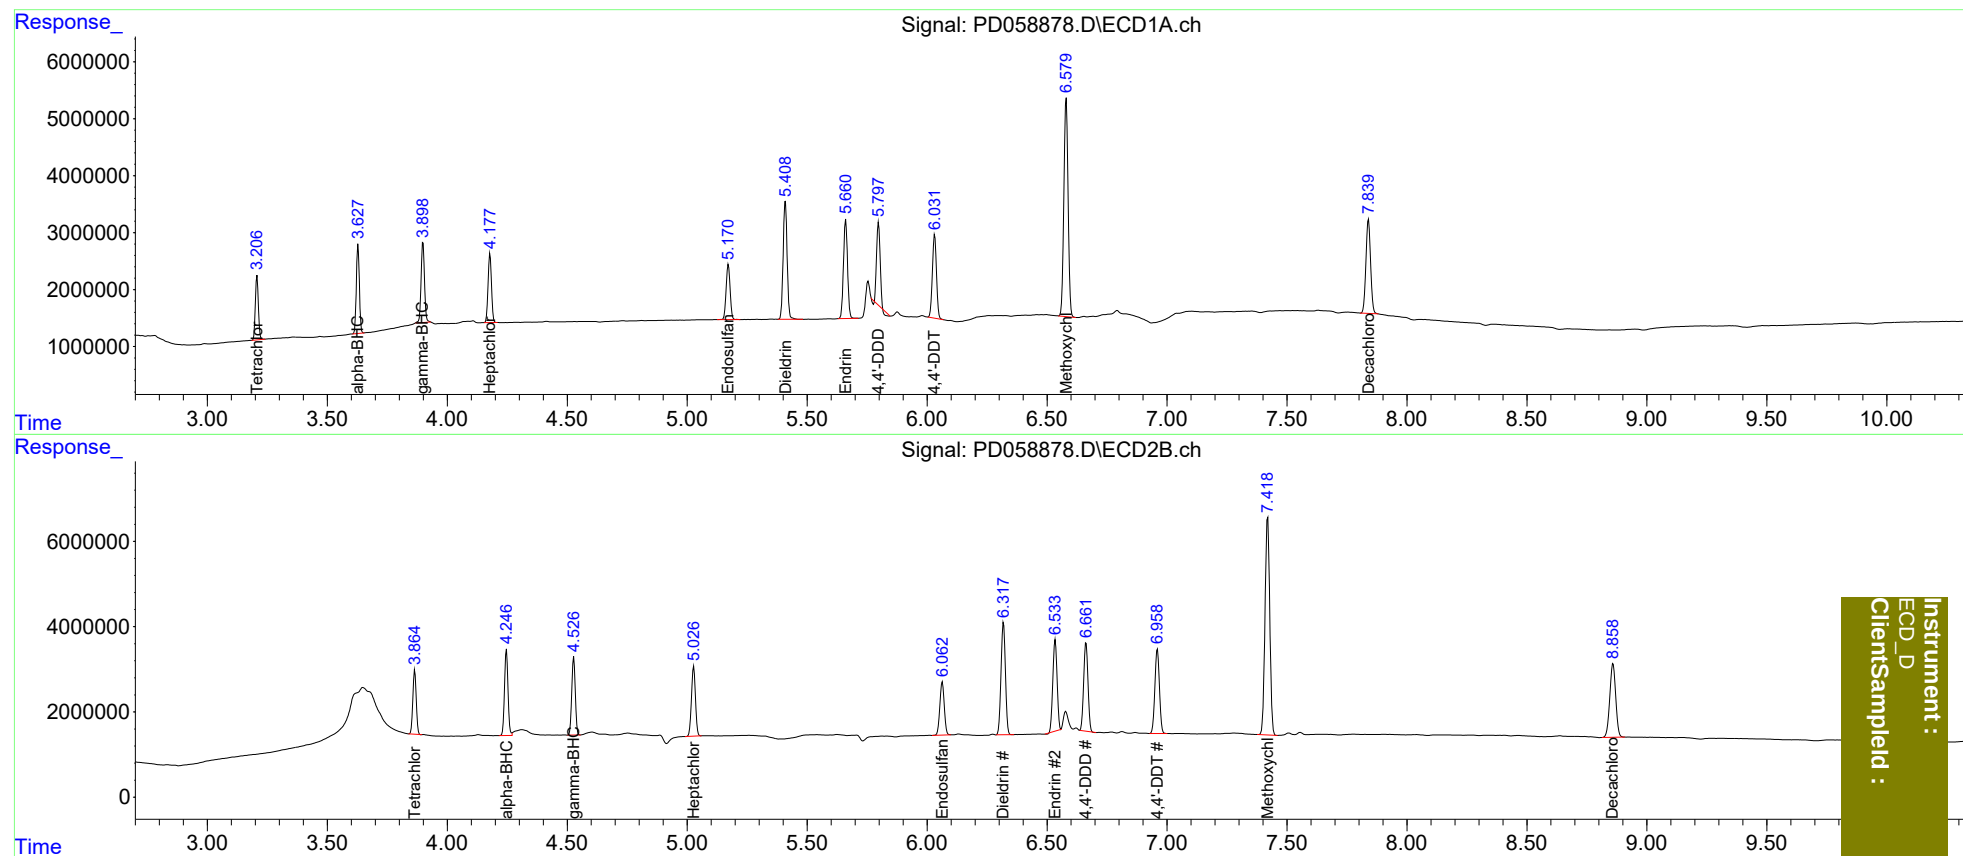


Instrument :
ECD_D
ClientSampled :

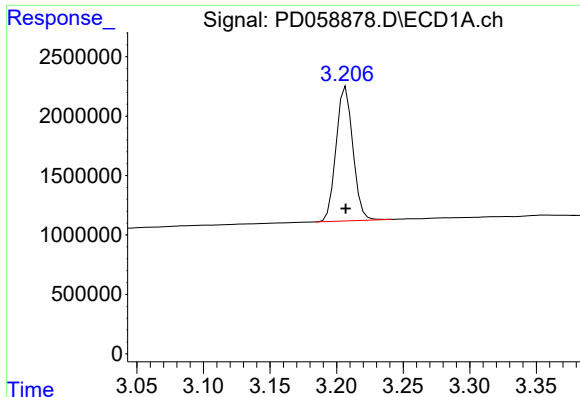

#1 Tetrachloro-m-xylene


R.T.: 3.207 min
Delta R.T.: 0.000 min
Response: 9951436
Conc: 10.16 ng/ml

Instrument :
ECD_D
ClientSampleId :

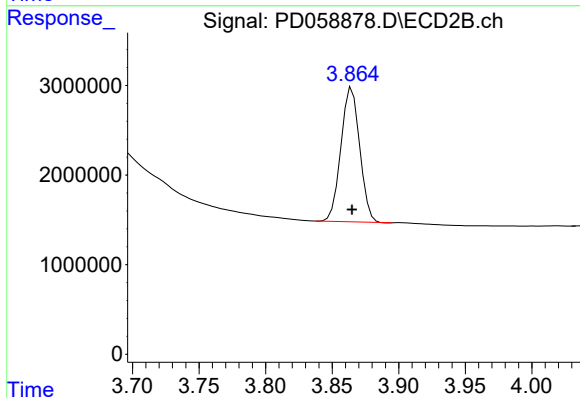


#1 Tetrachloro-m-xylene

R.T.: 3.865 min
Delta R.T.: 0.000 min
Response: 14697705
Conc: 9.90 ng/ml

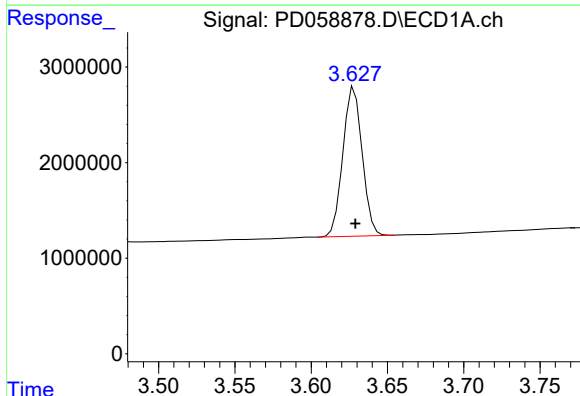


#2 alpha-BHC

R.T.: 3.628 min
Delta R.T.: 0.000 min
Response: 13733920
Conc: 9.67 ng/ml

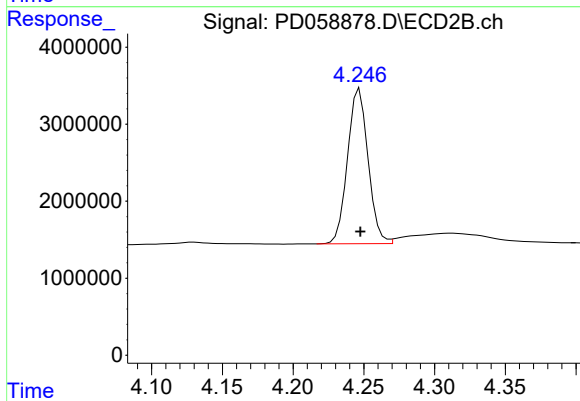

#2 alpha-BHC


R.T.: 4.247 min
Delta R.T.: 0.000 min
Response: 20410197
Conc: 9.74 ng/ml

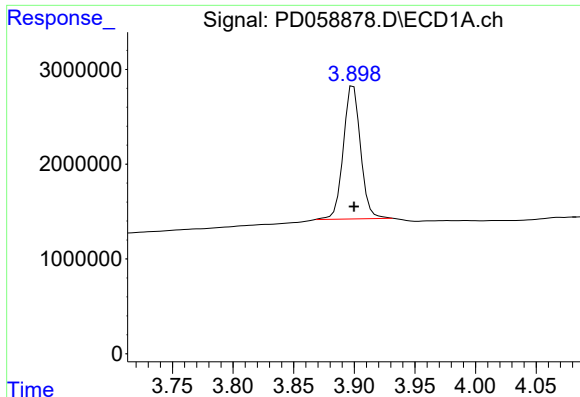

#3 gamma-BHC (Lindane)


R.T.: 3.899 min
Delta R.T.: 0.000 min
Response: 13882924
Conc: 10.11 ng/ml

Instrument :
ECD_D
ClientSampleId :

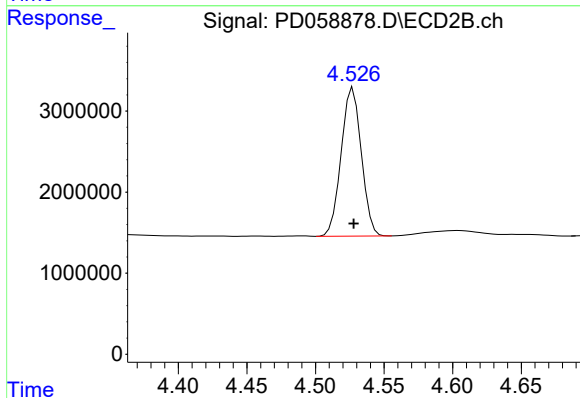


#3 gamma-BHC (Lindane)

R.T.: 4.527 min
Delta R.T.: 0.000 min
Response: 18761655
Conc: 9.61 ng/ml

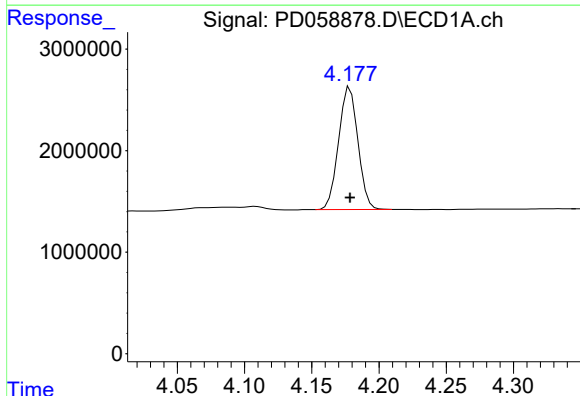


#4 Heptachlor

R.T.: 4.178 min
Delta R.T.: 0.000 min
Response: 12020511
Conc: 10.11 ng/ml

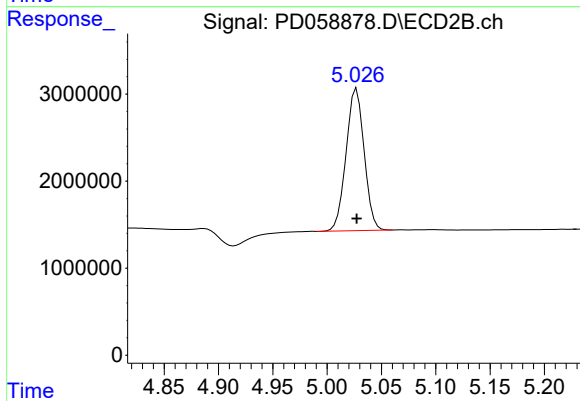

#4 Heptachlor


R.T.: 5.027 min
Delta R.T.: 0.000 min
Response: 18887001
Conc: 10.00 ng/ml

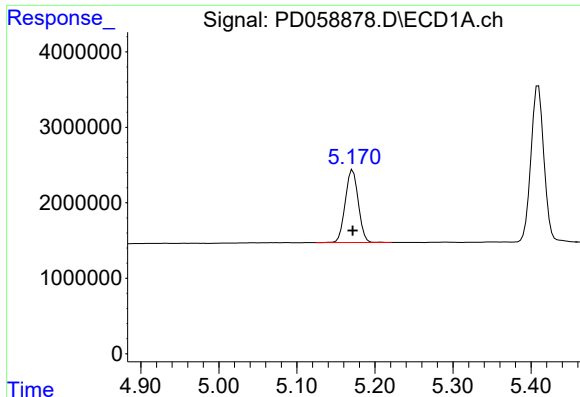

#9 Endosulfan I


R.T.: 5.172 min
Delta R.T.: 0.000 min
Response: 11160455
Conc: 10.18 ng/ml

Instrument :
ECD_D
ClientSampleId :

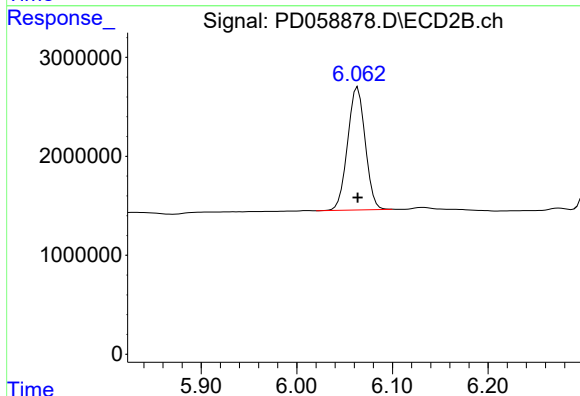


#9 Endosulfan I

R.T.: 6.064 min
Delta R.T.: 0.000 min
Response: 15949558
Conc: 10.13 ng/ml

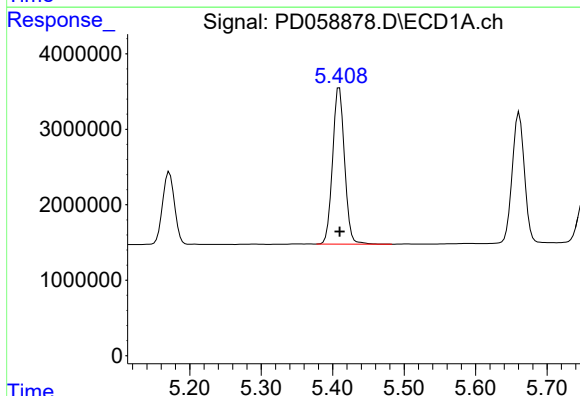


#13 Dieldrin

R.T.: 5.409 min
Delta R.T.: 0.000 min
Response: 24080190
Conc: 19.74 ng/ml

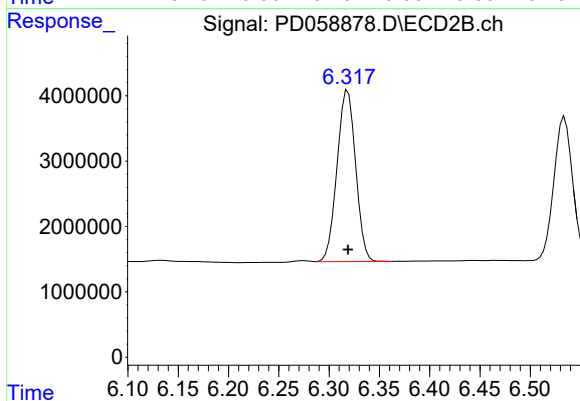

#13 Dieldrin


R.T.: 6.319 min
Delta R.T.: 0.000 min
Response: 33638396
Conc: 19.92 ng/ml

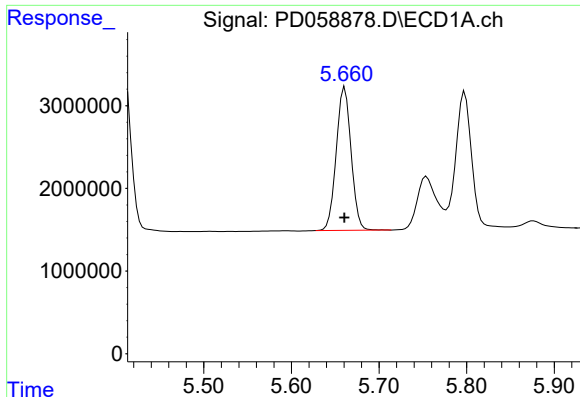

#14 Endrin


R.T.: 5.661 min
Delta R.T.: 0.000 min
Response: 20414933
Conc: 21.08 ng/ml

Instrument :
ECD_D
ClientSampleId :

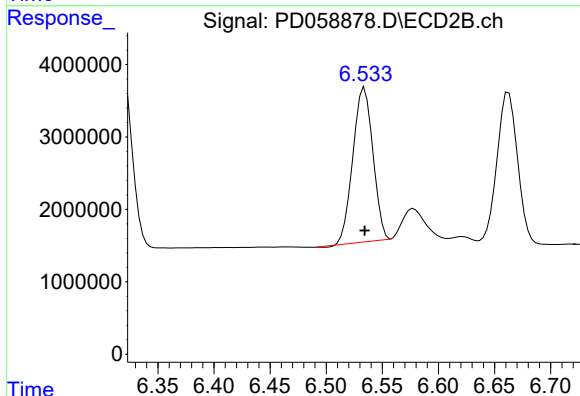


#14 Endrin

R.T.: 6.534 min
Delta R.T.: 0.000 min
Response: 26315693
Conc: 19.35 ng/ml

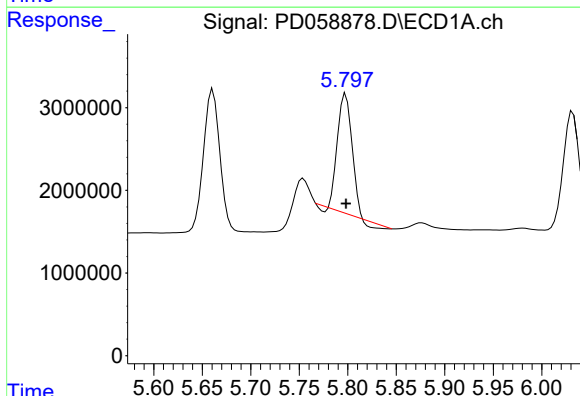


#16 4,4'-DDD

R.T.: 5.798 min
Delta R.T.: 0.000 min
Response: 14544108
Conc: 15.42 ng/ml

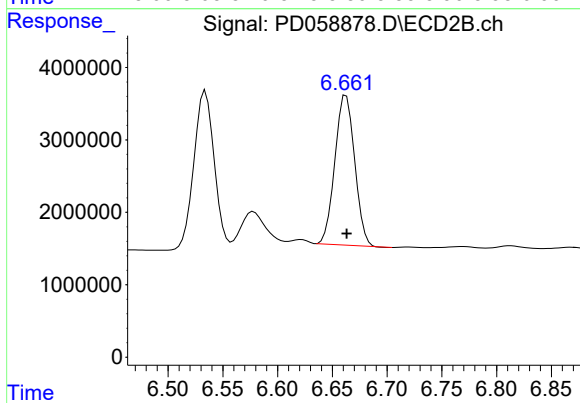

#16 4,4'-DDD


R.T.: 6.663 min
Delta R.T.: 0.000 min
Response: 26017690
Conc: 19.54 ng/ml

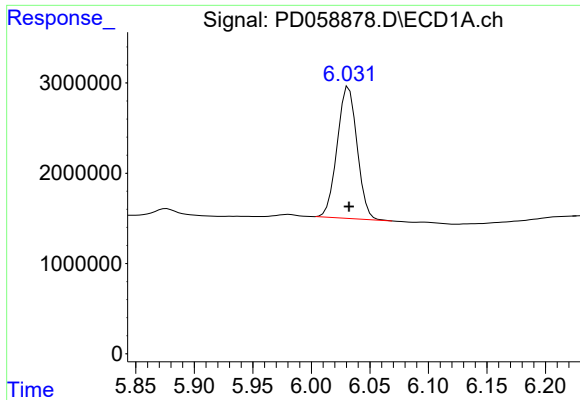

#17 4,4'-DDT


R.T.: 6.032 min
Delta R.T.: 0.000 min
Response: 17244552
Conc: 19.06 ng/ml

Instrument :
ECD_D
ClientSampleId :

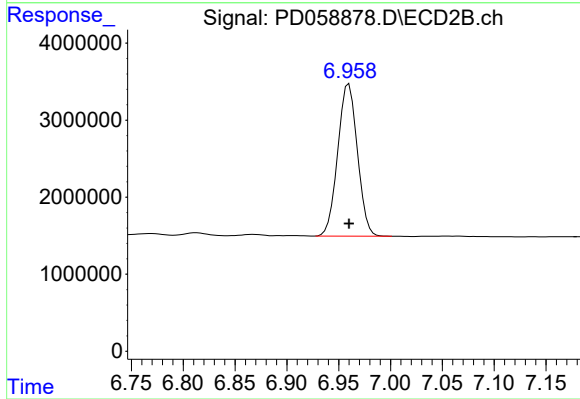


#17 4,4'-DDT

R.T.: 6.960 min
Delta R.T.: 0.000 min
Response: 26096171
Conc: 19.82 ng/ml

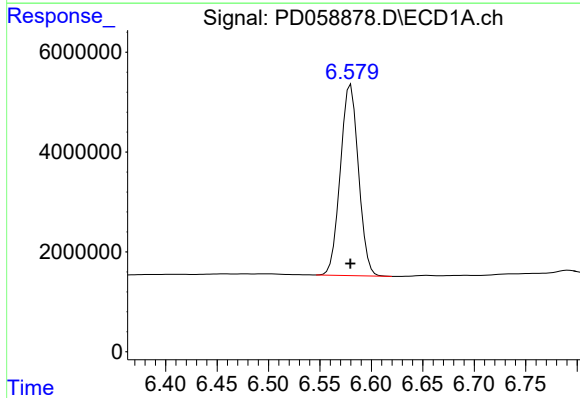


#20 Methoxychlor

R.T.: 6.580 min
Delta R.T.: 0.000 min
Response: 46988791
Conc: 103.92 ng/ml

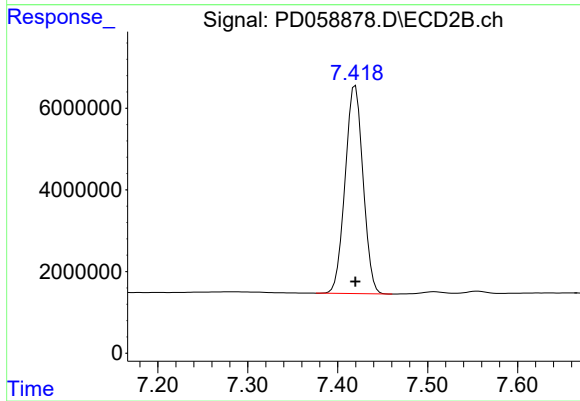

#20 Methoxychlor


R.T.: 7.420 min
Delta R.T.: 0.000 min
Response: 70514499
Conc: 101.69 ng/ml

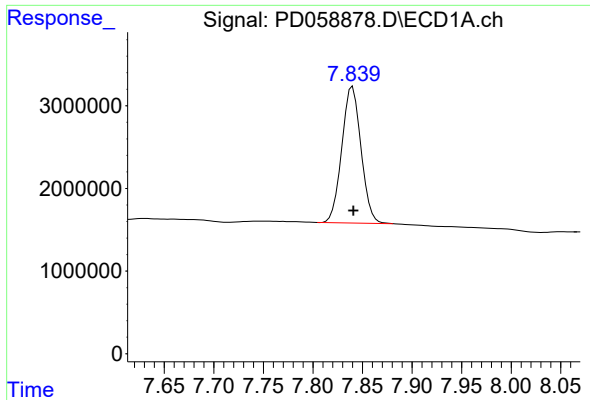

#27 Decachlorobiphenyl

R.T.: 7.840 min
Delta R.T.: 0.000 min
Response: 22230746
Conc: 20.88 ng/ml

Instrument :
ECD_D
ClientSampleId :

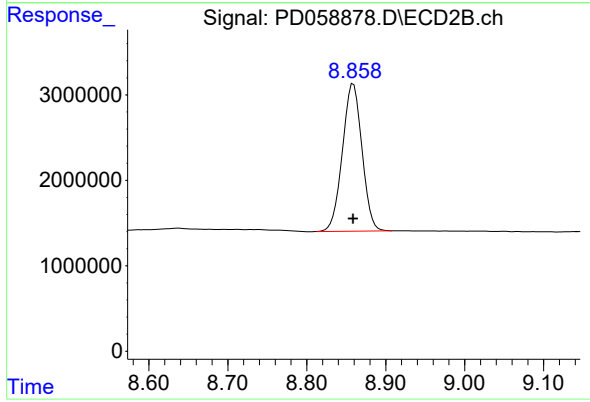

#27 Decachlorobiphenyl

R.T.: 8.859 min
Delta R.T.: 0.000 min
Response: 29726113
Conc: 21.72 ng/ml