

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080620\
 Data File : PD058880.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2020 08:22
 Operator : DD\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 09:19:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 06 09:11:39 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.207	3.865	19583183	29699420	20.000	20.000
27)	SA Decachlor...	7.841	8.858	42581206	54732950	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.629	4.248	28418409	41891696	20.000	20.000
3)	MA gamma-BHC...	3.900	4.528	27474869	39029443	20.000	20.000
4)	MA Heptachlor	4.179	5.027	23770269	37787331	20.000	20.000
9)	A Endosulfan I	5.172	6.064	21923366	31482671	20.000	20.000
13)	MA Dieldrin	5.410	6.319	48793754	67532799	40.000	40.000
14)	MA Endrin	5.661	6.534	38735242	54386588	40.000	40.000
16)	A 4,4'-DDD	5.798	6.663	37720432	53253436	40.000	40.000
17)	MA 4,4'-DDT	6.032	6.960	36195036	52655746	40.000	40.000
20)	A Methoxychlor	6.580	7.420	90429797	138.7E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080620\
Data File : PD058880.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2020 08:22
Operator : DD\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 09:19:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 06 09:11:39 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

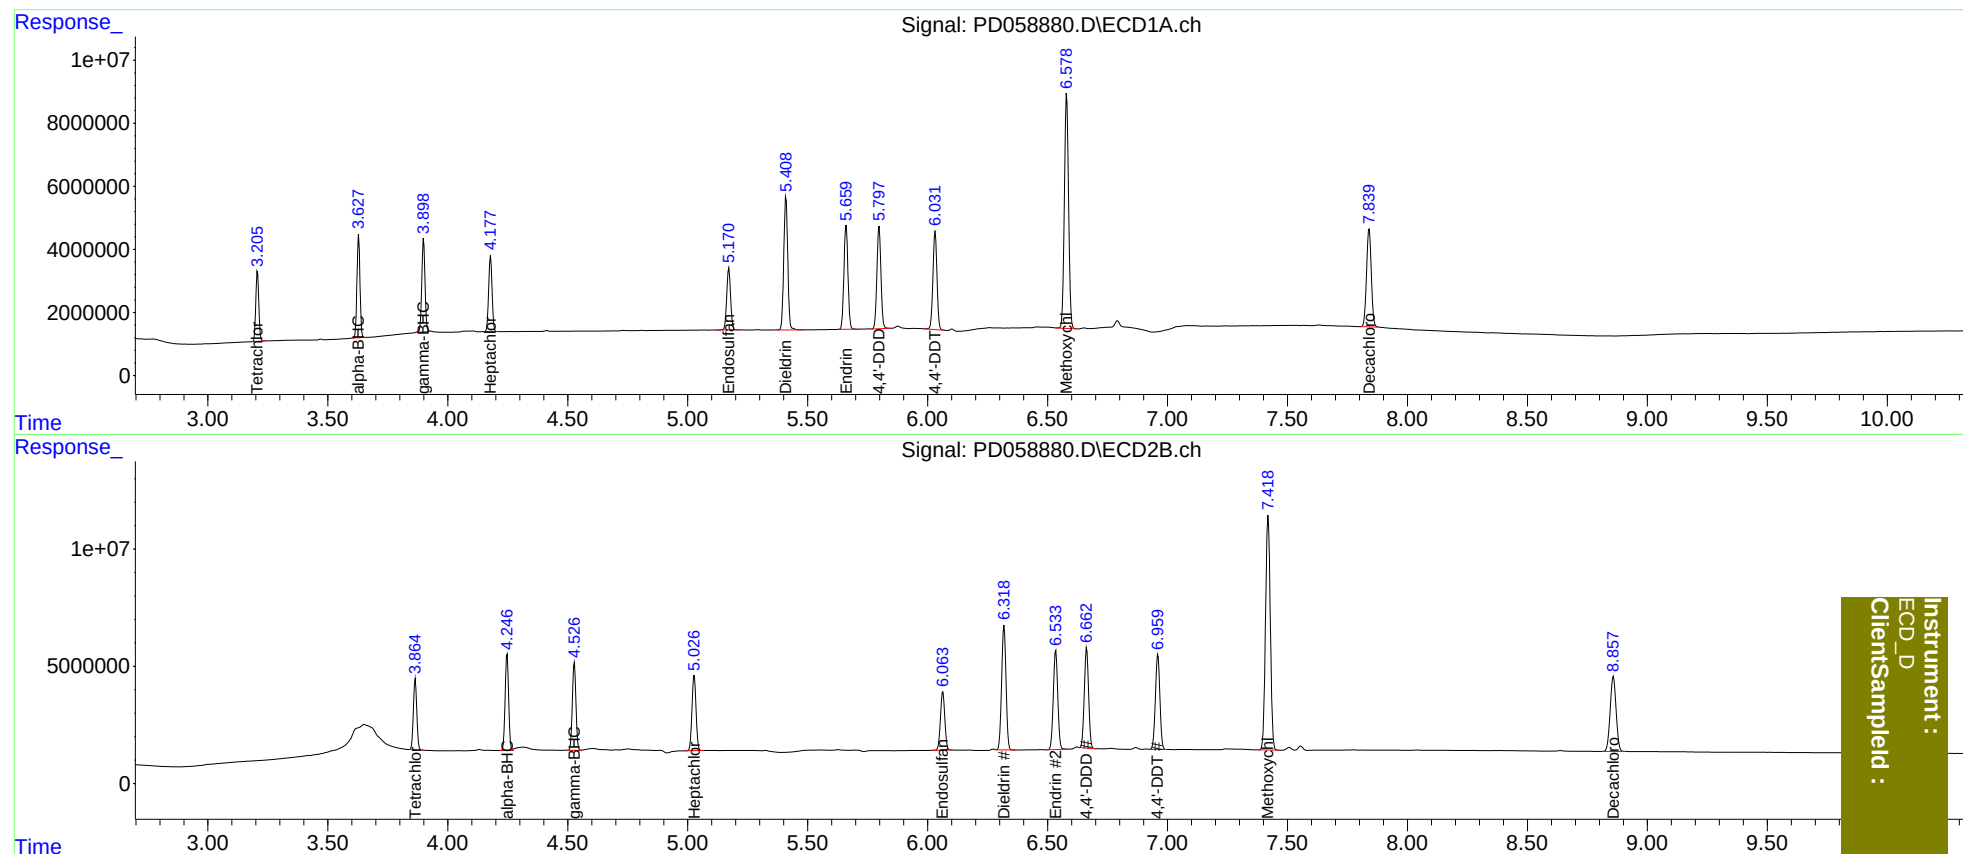


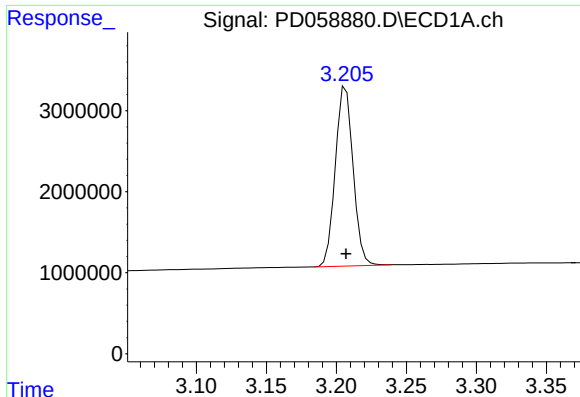

#1 Tetrachloro-m-xylene


R.T.: 3.207 min
Delta R.T.: 0.000 min
Response: 19583183
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

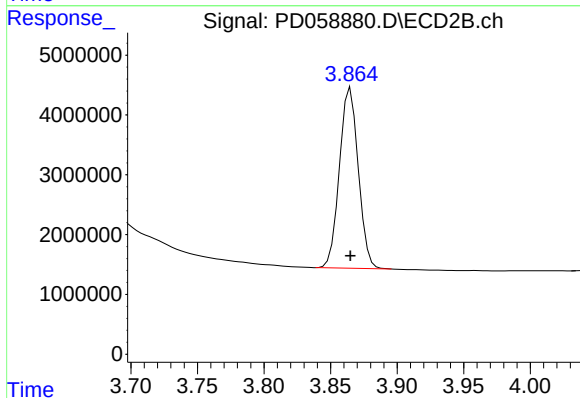


#1 Tetrachloro-m-xylene

R.T.: 3.865 min
Delta R.T.: 0.000 min
Response: 29699420
Conc: 20.00 ng/ml

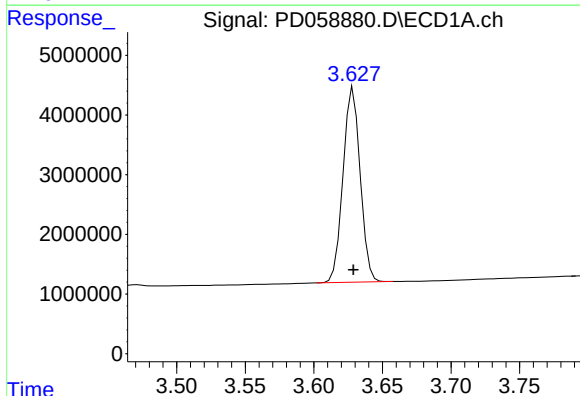


#2 alpha-BHC

R.T.: 3.629 min
Delta R.T.: 0.000 min
Response: 28418409
Conc: 20.00 ng/ml

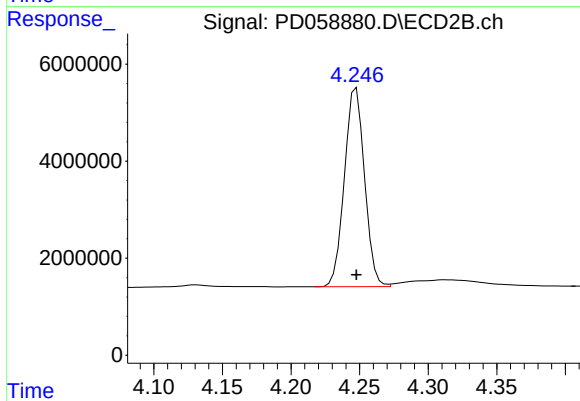

#2 alpha-BHC


R.T.: 4.248 min
Delta R.T.: 0.000 min
Response: 41891696
Conc: 20.00 ng/ml

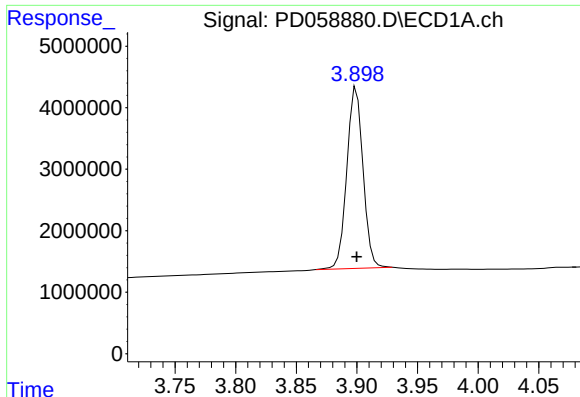

#3 gamma-BHC (Lindane)


R.T.: 3.900 min
Delta R.T.: 0.000 min
Response: 27474869
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

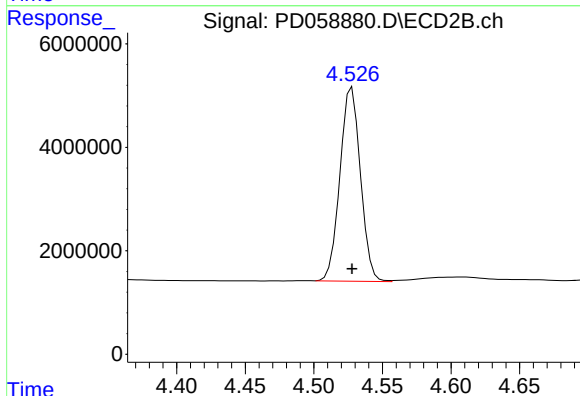


#3 gamma-BHC (Lindane)

R.T.: 4.528 min
Delta R.T.: 0.000 min
Response: 39029443
Conc: 20.00 ng/ml

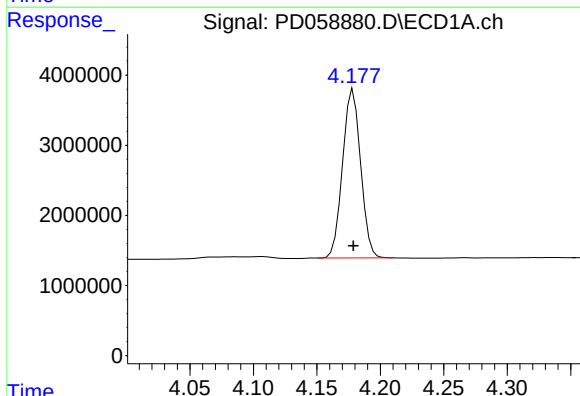


#4 Heptachlor

R.T.: 4.179 min
Delta R.T.: 0.000 min
Response: 23770269
Conc: 20.00 ng/ml

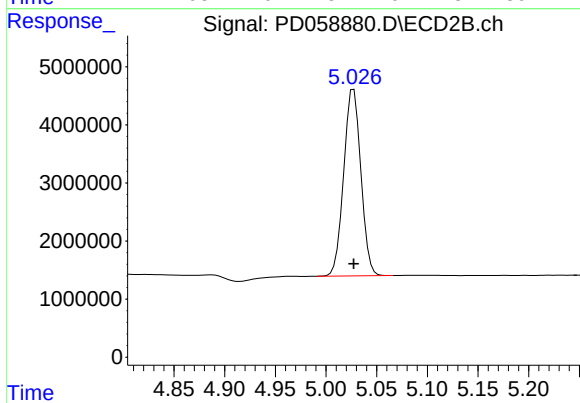

#4 Heptachlor


R.T.: 5.027 min
Delta R.T.: 0.000 min
Response: 37787331
Conc: 20.00 ng/ml

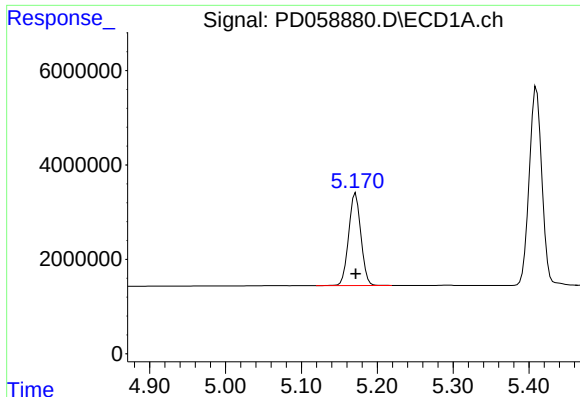

#9 Endosulfan I


R.T.: 5.172 min
Delta R.T.: 0.000 min
Response: 21923366
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

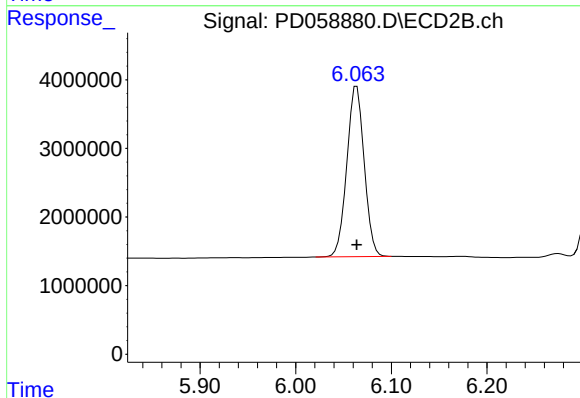


#9 Endosulfan I

R.T.: 6.064 min
Delta R.T.: 0.000 min
Response: 31482671
Conc: 20.00 ng/ml

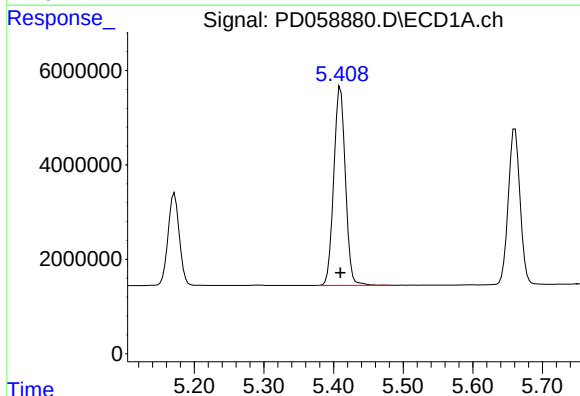


#13 Dieldrin

R.T.: 5.410 min
Delta R.T.: 0.000 min
Response: 48793754
Conc: 40.00 ng/ml

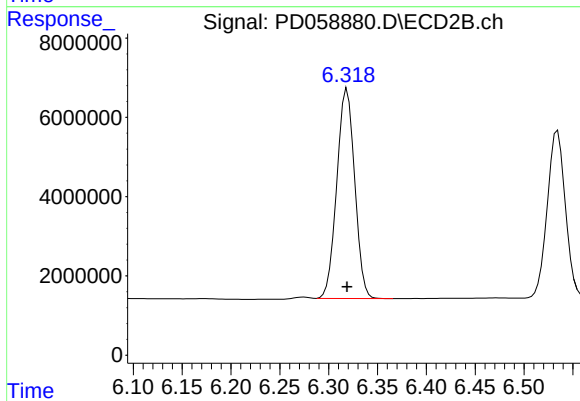

#13 Dieldrin


R.T.: 6.319 min
Delta R.T.: 0.000 min
Response: 67532799
Conc: 40.00 ng/ml

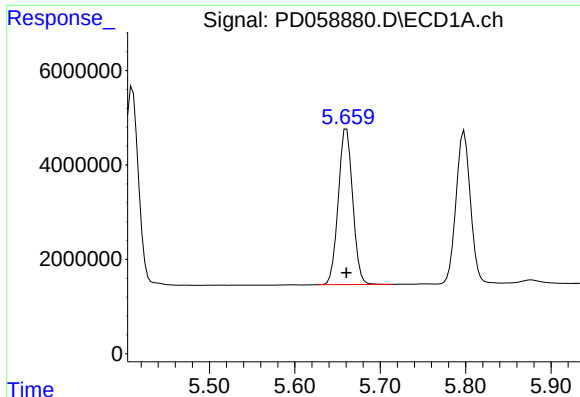

#14 Endrin


R.T.: 5.661 min
Delta R.T.: 0.000 min
Response: 38735242
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

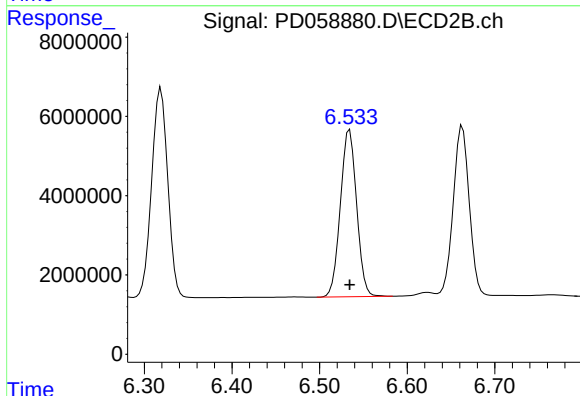


#14 Endrin

R.T.: 6.534 min
Delta R.T.: 0.000 min
Response: 54386588
Conc: 40.00 ng/ml

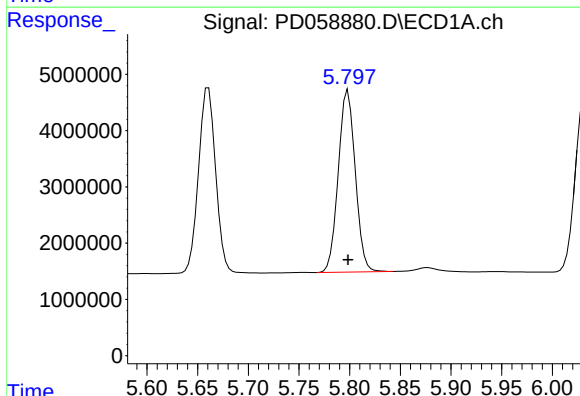


#16 4,4'-DDD

R.T.: 5.798 min
Delta R.T.: 0.000 min
Response: 37720432
Conc: 40.00 ng/ml

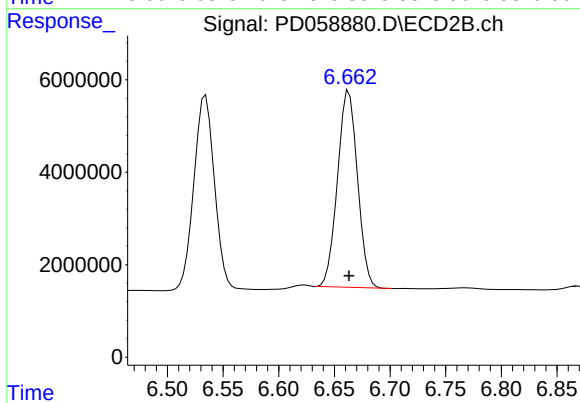

#16 4,4'-DDD


R.T.: 6.663 min
Delta R.T.: 0.000 min
Response: 53253436
Conc: 40.00 ng/ml

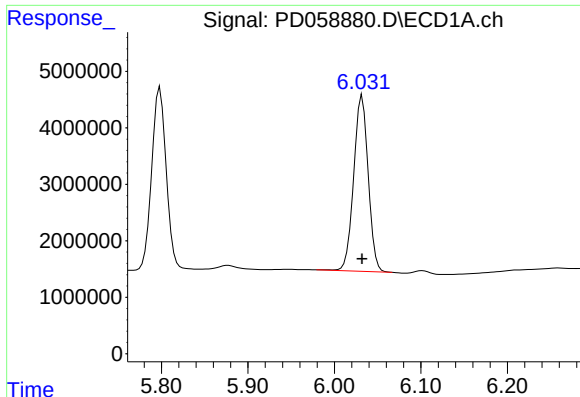

#17 4,4'-DDT


R.T.: 6.032 min
Delta R.T.: 0.000 min
Response: 36195036
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

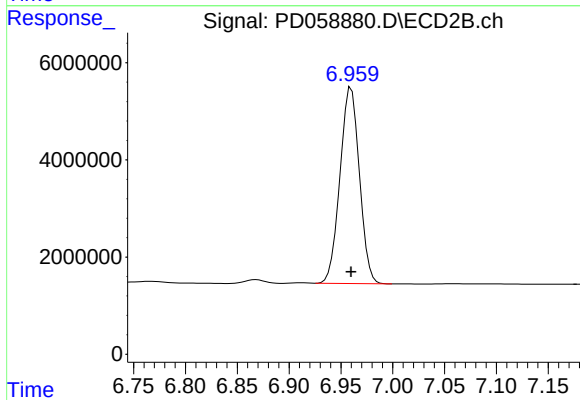


#17 4,4'-DDT

R.T.: 6.960 min
Delta R.T.: 0.000 min
Response: 52655746
Conc: 40.00 ng/ml

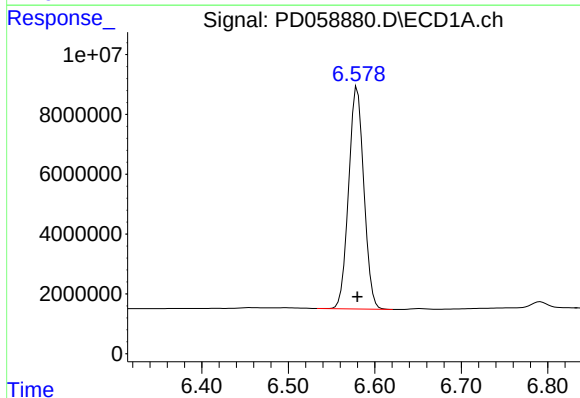


#20 Methoxychlor

R.T.: 6.580 min
Delta R.T.: 0.000 min
Response: 90429797
Conc: 200.00 ng/ml

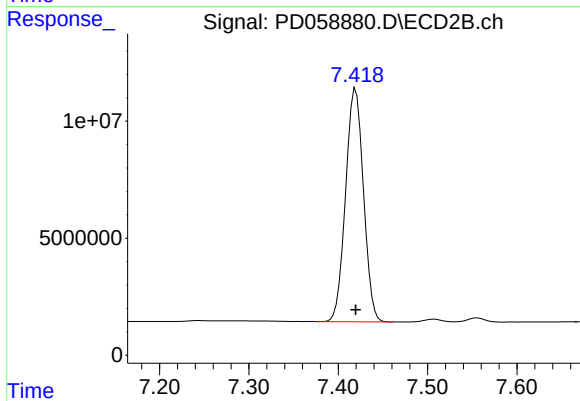

#20 Methoxychlor


R.T.: 7.420 min
Delta R.T.: 0.000 min
Response: 138686769
Conc: 200.00 ng/ml

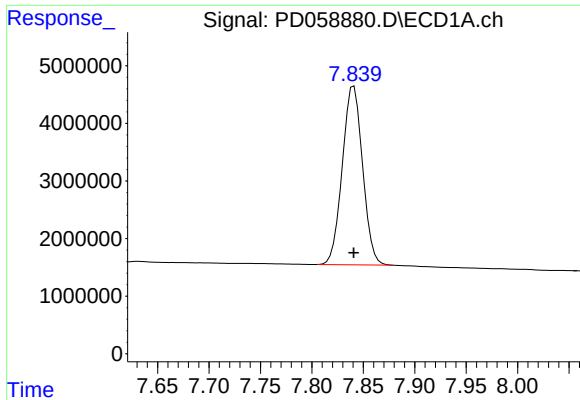

#27 Decachlorobiphenyl

R.T.: 7.841 min
Delta R.T.: 0.000 min
Response: 42581206
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

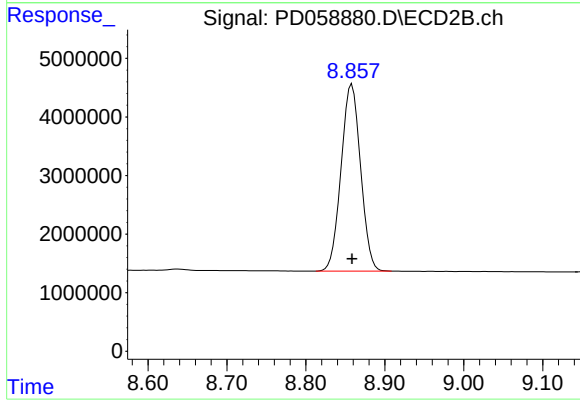

#27 Decachlorobiphenyl

R.T.: 8.858 min
Delta R.T.: 0.000 min
Response: 54732950
Conc: 40.00 ng/ml